A15

SERVICE MANUAL

ENGLISH

SERVICE MANUAL
English

TESE00005-05-ING
January - 2007

CE

TABLE OF CONTENTS

1. INTRODUCTION 9
1.1. GENERAL DESCRIPTION OF THE ANALYZER 9
1.1.1. Operating arm 10
1.1.2. Dispensing system 10
1.1.3. Reactions rotor and reading 11
1.1.4. Electronic system 12
1.1.5. Application program 12
1.2. FUNCTIONING OF THE ANALYSER 12
1.3. TRANSPORT AND RESHIPMENT OF THE ANALYZER 13
2. MECHANICAL ELEMENTS 15
2.1. Instrument breakdown 15
2.2. Description of the mechanical elements 16
2.2.1. Operating arm 16
2.2.1.1. X Guide. 17
2.2.1.2. X Carriage 18
2.2.1.3. Y Carriage 18
2.2.1.4. Needle unit 20
2.2.2. Dispensing system 21
2.2.2.1. Thermostated probe 21
2.2.2.2. Dispensing pump 22
2.2.2.3. Tubes and containers 23
2.2.2.4. Container level control sensors. 24
2.2.2.5. Racks tray with integrated washing station. 25
2.2.2.6. Washing pumps 26
2.2.3. Reaction rotor with integrated optical system. 26
2.2.3.1. Thermostated rotor and photometric system 26
2.2.3.2. Lighting system 29
2.2.4. Electronics cover 30
2.2.5. Main cover hinges 31
2.2.6. Base 32
2.2.7. Casings 33
3. Electronic system 34
3.1 CPU Board (CIIM00026) 34
3.2 Power Supply Board (CIIM00007-01) 39
3.3 Needle Board (CIIM00017) 41
3.4 Photometry Board (CIIM00027) 43
3.5 XYZ Interconnection Board (CIIM00018) 44
3.6 Communications Board (CIIM00036) 45
3.7 Rotor interconnection board (CIIM00029) 46
3.9 Pump interconnection board (CIIM00028) 48
3.10 Interconnection between boards 50
4. SERVICE PROGRAM 56
4.1 Initialising the analyser 56
4.2. ADJUSTMENTS 58
4.2.1. Adjustment of the needle thermostatation system 58
4.2.2. Adjustment of the rotor thermostation system 59
4.2.3. Adjustment of the positioning of the operating arm 60
4.2.3.1 Adjusting the maximum sweep of the Z axis. 60
4.2.4. Adjustment of the positioning of the rotor 62
4.2.4.1. Centering of the rotor with regard to the dispensing point 62

4.2.4.2. Centering of the rotor with regard to the optical system 62
4.2.5 . Adjustment of the positioning of the filter wheel 63
4.2.6. Adjustment of the level control scales 64
4.2.7. Adjustment of the level detection sensitivity 64
4.3. TESTS 65
4.3.1. Motor tests 66
4.3.1.1. Initialization test 66
4.3.1.2. Movement test 66
4.3.1.3. Loss step test 67
4.3.1.4. Stress mode test 67
4.3.1.5. Z axis security systems test 68
4.3.1.6 Maximum Z verification test 68
4.3.2. Diaphragm pumps and electrovalves test 69
4.3.2.1. Functioning test 69
4.3.2.2. Stress mode test 69
4.3.3. Needle self-centering system test 69
4.3.4. Needle level detection system test 70
4.3.5. Needle thermostatation system test 71
4.3.6. Needle rotor thermostatation system test 72
4.3.7. Photometry tests 72
4.3.7.1. Base line and integration times 72
4.3.7.2. Darkness counts 74
4.3.7.3. Repeatability without moving the filter wheel 75
4.3.7.4. Stability 75
4.3.7.5. Repeatability moving filter wheel 76
4.3.7.6. Absorbance measurement 77
4.3.7.7. Reactions rotor check 77
4.3.8. Level control scales test 78
4.3.9. Covers detection test 78
4.3.10. PC-Analyzer communications channel test 79
4.3.11. Global stress mode of the analyzer 79
4.4. UTILITIES 80
4.4.1. Disassembly of the dispensing needle 80
4.3.2. Fluid system supply 81
4.3.3. Cleaning of the dispensing system 82
4.3.4. Changing the lamp 82
4.3.5. Configuration of the filter wheel 83
4.3.6. Demonstration mode 84
4.4.7 Read/load adjustments and cycles 85
4.5. REGISTER 86
4.5.1. Introducing the analyzer serial number 86
4.5.2. Service Reports 86
4.5.3. Language change 87
4.5.4. Users 88
4.6. MONITOR 88
4.7 User's program 89
4.7.1 Configuration of the level of access to the analyser 89
4.7.2 Reagent Consumption 91
5. MAINTENANCE AND CLEANING 92
5.1. MAINTENANCE OPERATIONS 92
5.1.1. Housings and covers 92
5.1.1.1. Removing the needle unit casing 92
5.1.1.2. Removing the front housing 92
5.1.1.3. Removing the main cover 93
5.1.1.4. Removing the upper casing 94
5.1.1.5. Removing the spring protector 96
5.1.2. Operating arm 96

5.1.2.1. Fully removing the operating arm 96
5.1.2.2. Changing the arm hose 97
5.1.2.3. Changing the X motor 98
5.1.2.4. Changing the Y motor 100
5.1.2.5. Changing the Z motor 100
5.1.2.6. Changing the Y motor belt 101
5.1.2.7. Changing the spring 101
5.1.3. Dispensing system 102
5.1.3.1. Changing the thermostated pipe. 102
5.1.3.2. Changing the dispensing pump seal 103
5.1.3.3. Changing the dispensing pump motor 104
5.1.3.4. Changing the dispensing electrovalve 105
5.1.3.5. Changing the container tube unit 105
5.1.3.6. Changing the distilled water container filters 105
5.1.4. Reactions rotor and reading 106
5.1.4.1. Changing the rotor temperature probe 106
5.1.4.2. Fully removing the rotor 107
5.1.4.3. Changing the rotor Peltier cells 107
5.1.4.4. Changing the rotor cover detector 108
5.1.4.5. Changing the rotor start photosensor 109
5.1.4.6. Changing the rotor motor 110
5.1.4.8. Changing the lamp 110
5.1.4.9. Changing an optical filter 111
5.1.4.10. Configuration of the filter drum 112
5.1.4.11. Changing the filter drum start photosensor 113
5.1.4.12. Changing the filter drum motor 113
5.1.5. Electronic Systems 113
5.1.2.1. Changing the X, Y and encoder start photosensor 113
5.1.5.2. Changing the microprocessor board 113
5.1.5.3. Changing the power supply board 114
5.1.5.4. Changing the main power supply source 115
5.1.5.5. Changing the photometric system board 115
5.1.5.6. Changing the front indicator 116
5.1.5.7. Changing the firmware program 117
5.2. RECOMMENDED PREVENTIVE MAINTENANCE 117
5.3. CARE AND CLEANING 117
5.3.1. General care of the analyzer 117
5.3.2. Cleaning the optical system 118
5.3.3. Cleaning the dispensing system 118
5.3.4. General cleaning of the interior of the apparatus 118
A I. Technical specifications 119
A II. ADJUSTMENT MARGINS TABLES 123
A III. List of consumables, accessories and spares 124
A IV. LIST OF REQUIRED TOOLS 126
A V. SOFTWARE VERSIONS 126

1. INTRODUCTION

The ***A15*** analyzer is an automatic random access analyser specially designed for performing biochemical and turbidimetric clinical analyses. The instrument is controlled *on-line* in real time from an external dedicated PC.

In each of the elements of the A15 analyser, BioSystems has used leading edge technology to obtain optimum analytical performance, as well as taking into account economy, robustness, easy use and maintenance. A three-axis Cartesian operating arm prepares the reactions. Dispensing is performed by means of a pump with a ceramic piston via a detachable thermostated needle. A washing station guarantees that the needle is kept perfectly clean throughout the process. The reactions take place in a thermostated rotor in which absorbance readings are taken directly by means of an integrated optical system.

This manual contains the information required for learning about, maintaining and repairing the ***A15*** automatic analyzer. It should be used by the Technical Service as a learning and consultation document for the maintenance and repair of the instrument. Chapter 2 describes the different mechanical elements that form the analyzer together with their functionality, and chapter 3 describes the electronic system. Chapter 4 describes the Service Program. All the adjustments and checks of the analyzer are carried out through this program, which is independent from the application program (User Program). The separation of both programs enable it to be maintained separately and the extensions and improvements of one do not affect the other. The user does not have the service program. The Technical Service must install it on the user's computer in order to carry out the service requirements. Once said tasks have been carried out, the Technical Service must uninstall the program. Chapter 5 offers instructions for the different maintenance, repair and cleaning operations that can be carried out by the Technical Service. The annexes contain a summary of the technical specifications of the analyzer, the adjustment margin tables, the lists of accessories and spares, a list of software versions and their compatibility and a software troubleshooting guide.

1.1. GENERAL DESCRIPTION OF THE ANALYZER

The ***A15*** analyser is made up of three basic elements: the operating arm, the dispensing system and the reading and reactions rotor. The electronic system of the instrument controls said elements and communicates with the external computer containing the application program. Through this program, the user can control all the operations of the analyzer.

1.1.1. Operating arm

This is a three-axis XYZ Cartesian mechanism. The X and Y axes move the dispensing needle over the analyser horizontally and the Z axis moves it vertically. It is operated by three step-by-step motors. In each 24-second preparation cycle, the operating arm performs the following actions: first of all, it sucks in the reagent from the corresponding bottle. Next, the needle is washed externally in the washing station and sucks in the sample from the corresponding tube. It is washed externally again and dispenses the sample and the reagent into the reactions rotor. Finally, it is exhaustively washed internally and externally before proceeding with the next preparation. The arm has a system for controlling vertical movement to detect whether or not the needle has collided into anything on descending. If a collision occurs, as may be the case if, for example, a lid has been left on a bottle of reagent, the arm automatically restarts, verifies the straightness of the needle and continues working issuing the corresponding alert to the user. A vertical axis retention system prevents the needle from falling in the case of a power cut, avoiding injury from the needle to the user or the needle being bent by an attempt to move the arm manually. The operating arm only makes the preparations if the general cover of the analyser is closed. If the cover is raised while it is functioning, the arm automatically aborts the task in progress and returns to its parked position to avoid injury to the user.

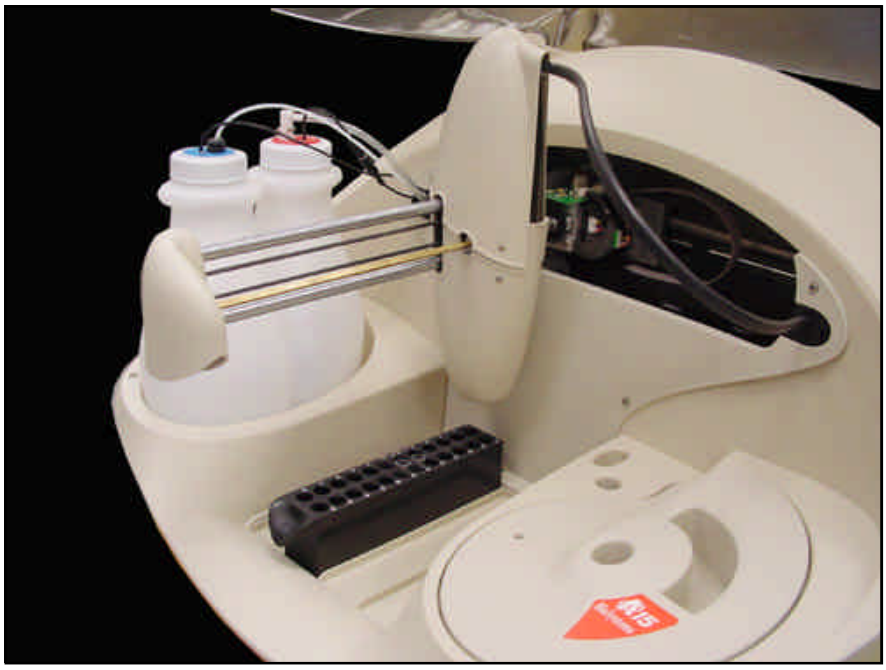

1.1.2. Dispensing system

This system consists of a thermostated needle, supported and displaced by an operating arm and connected to a dispensing pump. The needle is detachable to enable cleaning and replacement. The analyser has capacity level detection to control the level of the bottles and tubes and prevent the needle from penetrating too far into the corresponding liquids, thus minimising contamination. An automatic adjustment system informs the user if the needle is not mounted or if it is too bent. The needle has a sophisticated Peltier thermostatation system, with *PID* control, capable of thermostating the preparations at approximately 37º in less than 15 seconds. Dispensing is carried out by means of a low maintenance ceramic piston pump driven by a step-by-step motor. It is capable of dispensing between 3 and 1250 ml. The exterior of the needle is kept constantly clean by a wash station included in the base. A membrane pump transports the waste to the corresponding container.

The ***A15*** analyser has a tray with 4 free positions for racks of reagents or samples. Each reagents rack can carry up to 10 reagents in 20 ml or 50 ml bottles. Each samples rack can contain up to 24 tubes of samples. The samples can be patients, calibrators or controls. The analyser can be configured to work with 13 mm or 15 mm diameter tubes of samples with a length of up to 100 mm or with paediatric wells. Any possible configuration of racks can be mounted from 1 rack of reagents (10 reagents) and 3 racks of samples (72 samples) to 3 racks of reagents (30 reagents) and 1 rack of samples (24 samples).

On the left of the analyser are the waste and distilled water containers. The analyser constantly controls the level of these containers and issues the appropriate alerts if the distilled water is nearly empty or if the waste container is full.

1.1.3. Reactions rotor and reading

The preparations are dispensed in an optical quality methacrylate reactions rotor thermostated at 37ºC. The optical absorbance readings are taken directly on this rotor. Each reaction can be read for 10 minutes. The readings are taken as they are programmed in each measurement procedure. The reaction wells have been designed to enable the mixture of the sample and the reagent during the dispensing. Each rotor has 120 reaction wells. The length of the light path is 6 mm. The minimum volume required to take the optical reading is 200 uL. The wells have a maximum useful capacity of 800 uL. When the reactions rotor is completely full, the user must change it for one that is empty, clean and dry. The reactions rotors can be reused up to 5 times if they are carefully cleaned immediately after use. The *Cleaning the semi-disposable reactions rotor section* in the Installation and maintenance manual describes how to clean the rotors. The user has a test in the computer programme, which he or she may use to check the condition of the rotor. The rotor is driven by a step-by-step motor with a transmission. A Peltier system with PID control thermostates the rotor at 37ºC.

An optical system integrated in the rotor takes the readings directly on the reaction wells. The light source is a 10 W halogen lamp. The detector is a silicon photodiode. The wavelength is selected by a drum with 9 positions available for optic filters. The filters are easily changed by the user from the exterior of the analyser, without the need for disassembling the filter drum. A step-by-step motor positions the drum. The optical system is capable of taking 1.25 readings per second, with or without a filter change in between. The light beam from the lamp passes through a compensated interferential filter to select the desired wavelength. It then passes through the rotor well and finally reaches the photodiode, where the light signal is turned into an electric signal. A sophisticated analogical digital integrator-converter system converts the electric signal into a digital value with which the analyser obtains the absorbance values. The optical system continues to work when the general cover of the analyser is open, whereby the analyser can continue to take readings while the user handles, for example, the sample tubes or the reagent bottles. The rotor cover must be in place for the optical system to work correctly.

A detector tells the analyser of the presence of the cover. The analyser aborts the readings if the user removes the rotor cover while the optical system is taking photometric measurements. If the rotor is not covered, the analyser informs the user so that he or she places the rotor cover when it sends samples to be analyzed.

1.1.4. Electronic system

The described elements are controlled by an electronic system based on a microprocessor. The microprocessor has two external communication channels to connect the instrument to the computer containing the application program. The electronic system is made up of the following independent boards:

- Microprocessor board
- Photometric system board
- Needle conditioning board
- Fluid system interconnection board
- Arm interconnection board
- Rotor interconnection board
- Power supply board

1.1.5. Application program

The application program makes it possible to control all the operations of the analyzer. From this program, the user can monitor the state of the analyzer and the work session, program parameters, e.g. technique parameters, prepare the work session, prepare results reports, configure different analyzer options, activate various test utilities, prepare and maintain the instrument and carry out internal quality control processes. The purpose of this manual is not to explain the functioning of the user program. For detailed information to this regard, please consult the User Manual included with the analyzer.

1.2. FUNCTIONING OF THE ANALYSER

The ***A15*** analyser is an automatic random access analyser specially designed for performing biochemical and turbidimetric clinical analyses. The analyser performs patient-by-patient analyses and enables the continual introduction of samples. The analyser is controlled from a dedicated PC that is permanently communicated to the instrument. The programme, installed on the computer, keeps the user constantly informed of the status of the analyser and the progress of the analyses. As results are obtained, the computer shows them to the user immediately.

When a *Work Session* is begun, the analyser proposes performing the blanks, calibrators and controls programmed for the measurement procedures it is to carry out. The user may choose between performing the blanks and the calibrators or not. If they are not performed, the analyser uses the last available memorised data. The controls can also be activated or not. During a session, while the analyser is working, the user can introduce new normal or urgent samples to be analyzed. Each time a new sample is added, the analyser automatically proposes the possible new blanks, calibrators or controls to be performed. A work session can remain open for one or more days. When a session is closed and another new session is opened (Reset Session), the analyser again proposes performing the blanks, calibrators and controls. It is recommended that the session is reset each working day.

The analyser determines the concentrations of the analytes based on optical absorbance measurements. To measure the concentration of a certain analyte in a sample, the analyser uses a pipette to take a specific volume of the sample and the corresponding reagent, quickly thermostates them in the needle itself and dispenses them into the reactions rotor. The very dispensing speed together with the geometry of the reaction well causes the mixture to be shaken and the chemical reaction begins. In the bireagent modes, the reaction begins when the analyser later dispenses a second reagent in the same reaction well. The reactions can be biochemical or turbidimetric. In both cases, the reaction or the chain of reactions produced generate substances that attenuate certain wavelengths, either by absorption or by dispersion. Comparing the light intensity of a certain wavelength that crosses a well when there is a reaction and when there is not a reaction can determine the concentration of the corresponding analyte. This comparison is quantified with the physical magnitude called *absorbance*. In some cases, the concentration is a direct function of the absorbance, and in other cases, it is a function of the variation of the absorbance over time, depending on the analysis mode.

1.3. TRANSPORT AND RESHIPMENT OF THE ANALYZER

If the analyser is to be reshipped or moved using a transport vehicle, it is important to block the operating arm and use the original packaging to ensure that the apparatus is not damaged. To package the instrument, we recommend you follow the following instructions: (on the unpackaging instructions sheet)

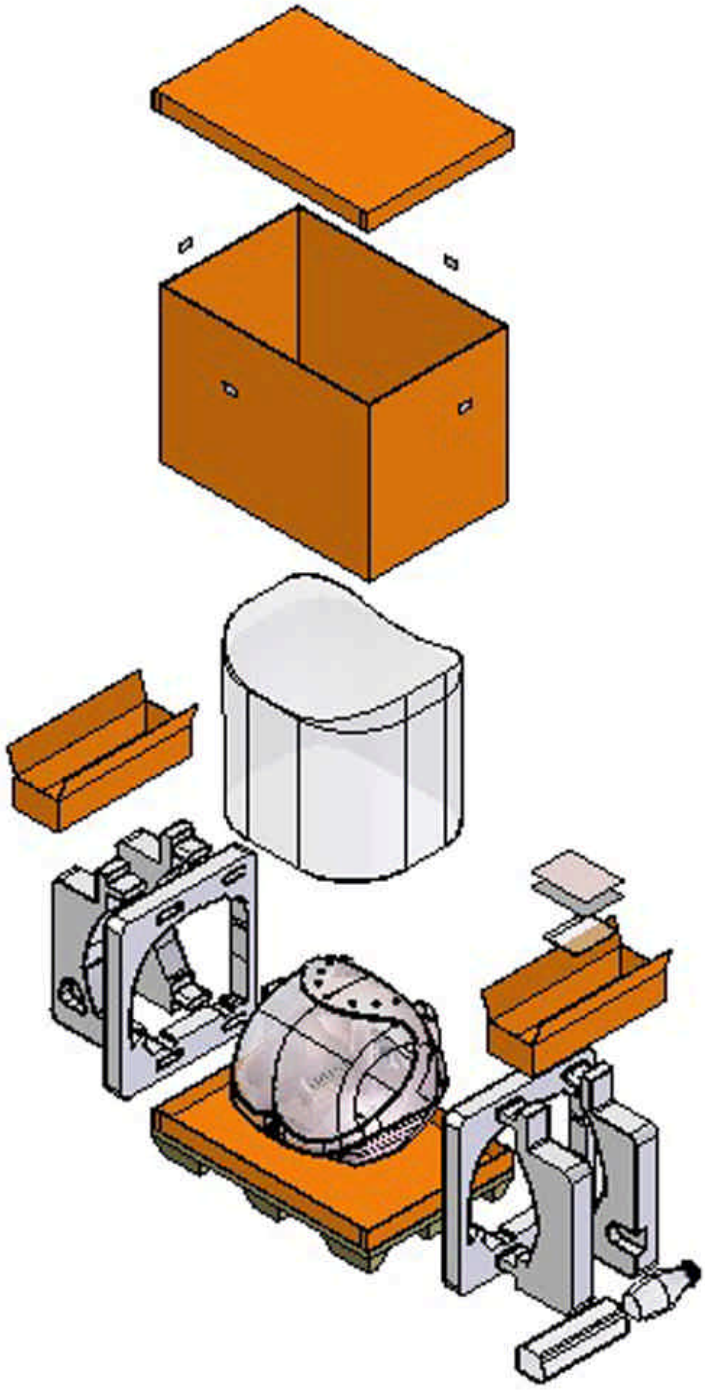

2. MECHANICAL ELEMENTS

2.1. Instrument breakdown

The physical structure of the analyzer can be broken down as follows:

-Operating arm
- -X guide.
- -Y guide.
- -X carriage.
- -Y carriage.
- -Needle unit.

-Dispensing system.
- -Thermostated probe.
- -Dispensing pump.
- -Tubes and containers.
- -Container level control sensors.
- -Racks tray with integrated washing station.
- -Waste pump.

-Reactions rotor with integrated optical system.
- -Thermostated rotor and photometric system. This contains the electronic photometric system board.
- -Lighting system.

-Electronics box.This houses the electronic boards of the microprocessor, the power supply and the front indicator.

-Main cover hinges.

-Base.

-Housings.
- -Upper casing.
- -Front housing.
- -Arm casing.
- -Main cover.

The following is a brief description of each of the mechanical elements that make up the analyzer.

2.2. Description of the mechanical elements

2.2.1. Operating arm

This mechanism positions the dispensing needle appropriately during the preparation of the analyses. An encoder checks the vertical movement of the needle and a spring automatically stops it from falling in the case of a power cut. The dispensing pipe and the electrical hoses of the arm pass through the front casing

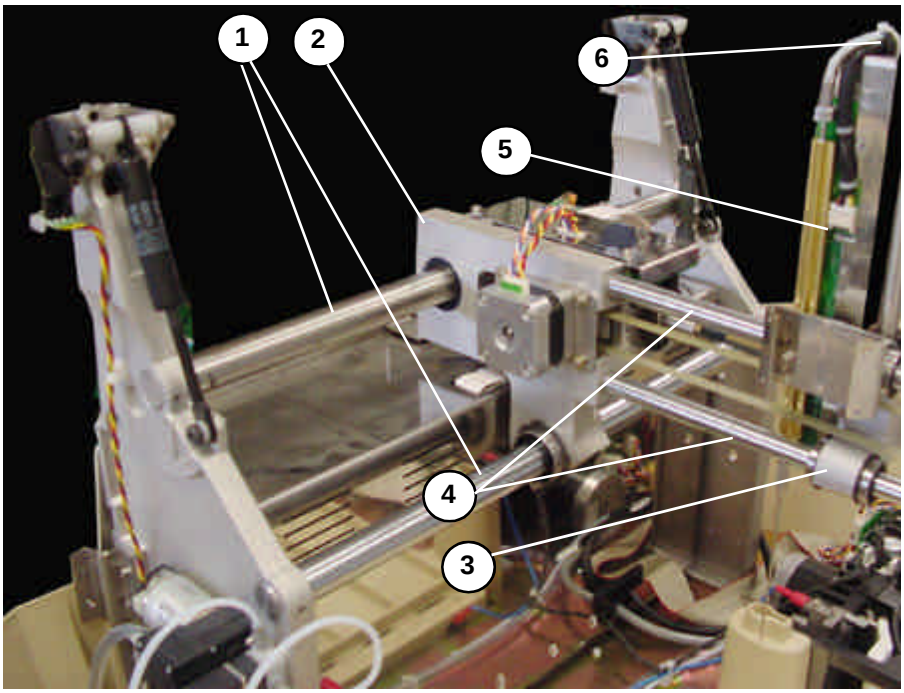

(1) X GUIDE
(2) X CARRIAGE
(3) Y CARRIAGE
(4) Y GUIDE.
(5) NEEDLE UNIT
(6) CONTROL AND DISPENSING PIPE HOSE

The needle unit (5) supports the thermostated needle and can move on the Y carriage (3), which can move on the Y axes (4). The Y axes are supported by the X carriage, which moves on the X axes (1). In this way, the needle can be moved in the three Cartesian directions of X, Y and Z. The hose (6) houses the Teflon dispensing tube and all the electrical hoses of the arm.

2.2.1.1. X Guide.

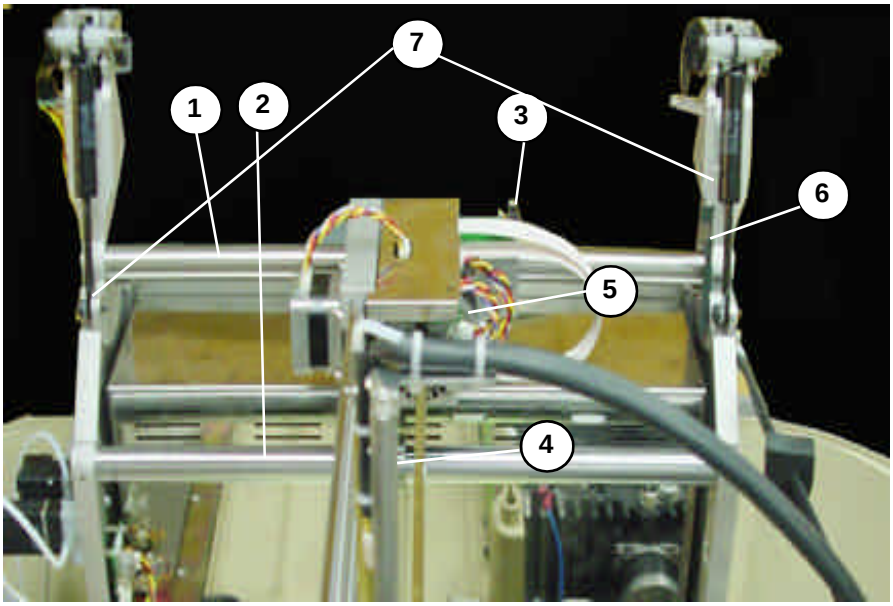

(1) UPPER X TOOTHED AXIS
(2) LOWER X AXIS
(3) X START PHOTOSENSOR
(4) BEARING
(5) X MOTOR
(6) X START PHOTOSENSOR TAB
(7) AXIS SUPPORTS

This consists of two supports (7) that hold the steel axes (1 and 2) on which the X carriage moves. The photosensor (3) indicates the start position of the X carriage movement. The motor (5) is moved by a rack (2). The X carriage is supported by the second axis (2) by means of a bearing (4).

2.2.1.2. X Carriage

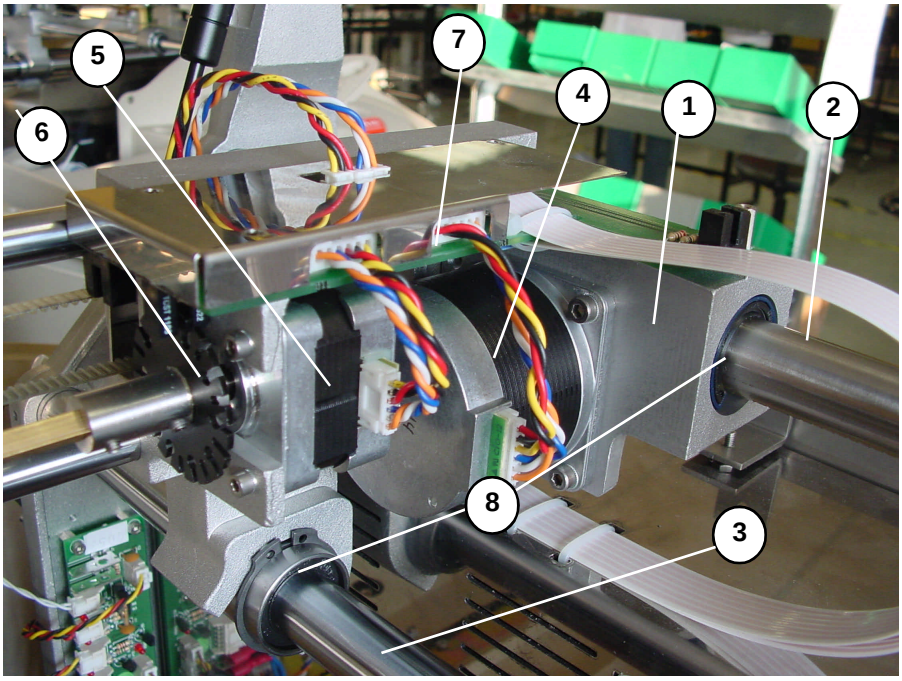

(1) X CARRIAGE BODY
(2) UPPER X AXIS - RACK
(3) LOWER X AXIS
(4) X MOTOR
(5) Z MOTOR
(6) ENCODER
(7) XYZ INTERCONNECTION PCB
(8) BEARINGS

The X carriage body (1) moves along the two axes (2, 3). The upper axis (2) acts as a rack. The X motor (4) is fitted with a pinion that moves the carriage. The X carriage also supports the interconnection PCB (7) and the Z motor (5). To enable the movement, it uses linear bearings (8).

2.2.1.3. Y Carriage

(1) Y CARRIAGE BODY
(2) Y GUIDE AXES
(3) Y MOTOR
(4) BELT
(5) BELT RETURN PULLEY
(6) START PHOTOSENSOR
(7) START TAB
(8) NEEDLE UNIT
(9) BEARINGS

The body of the Y carriage (1) moves along the two axes (2) on linear bearings (9). The said axes are supported by the X carriage. The movement is made by the Y motor (3) by the belt (4) and the return pulley (5). The start of the movement is controlled by the tab (7) and the start photosensor (6) located on the X carriage (10). The body of the Y carriage (1) also supports the needle unit.

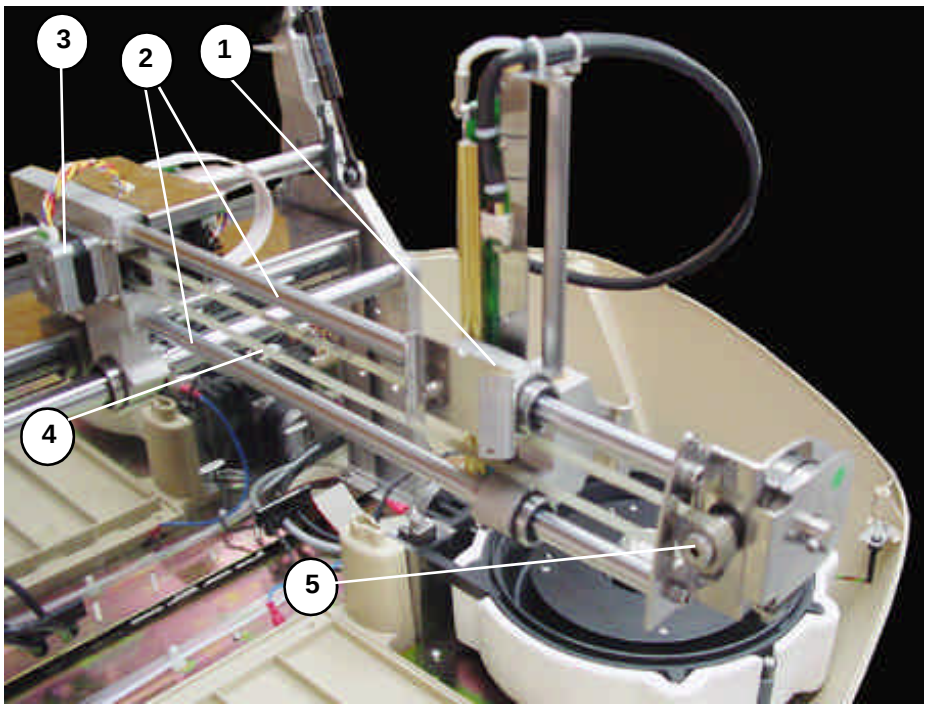
3
2
1
4
5

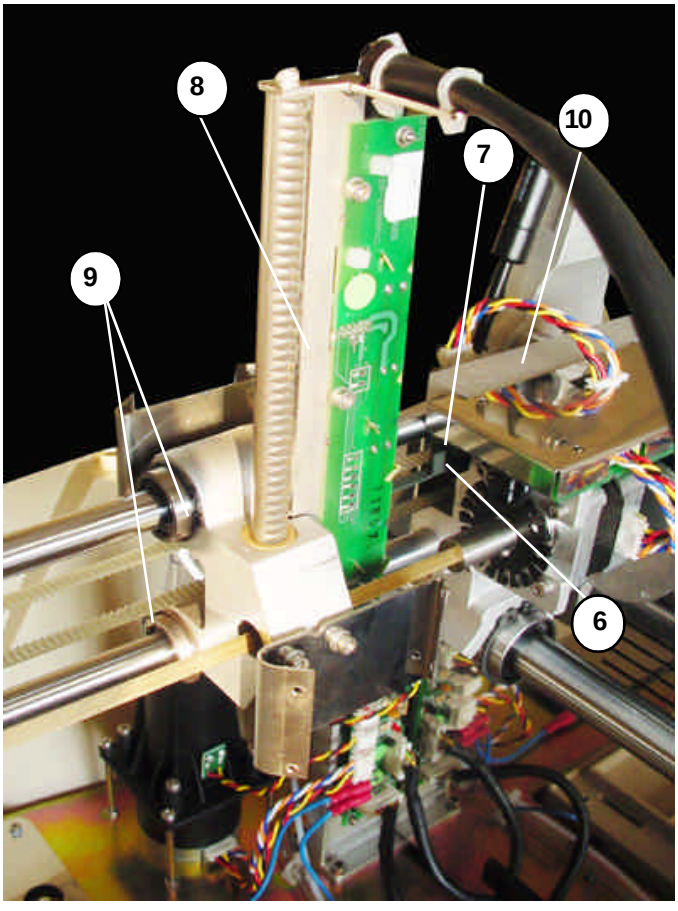
8
10
7
9
6

2.2.1.4. Needle unit

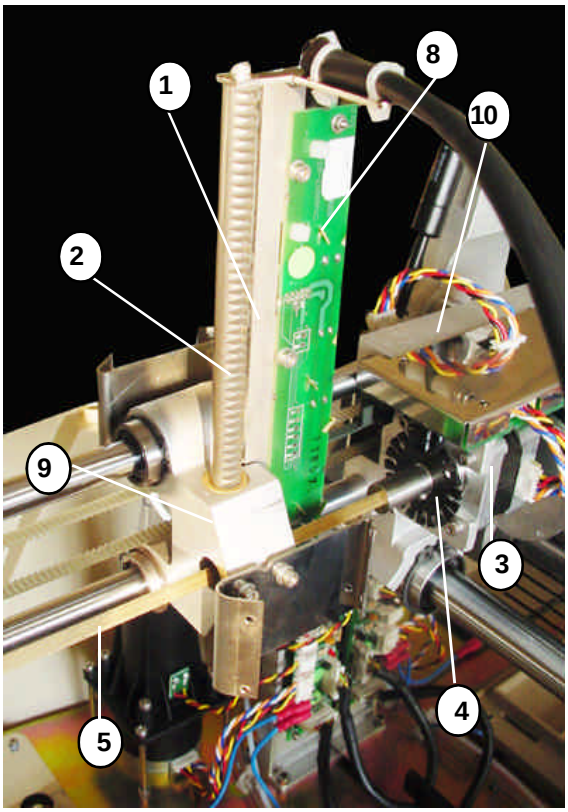

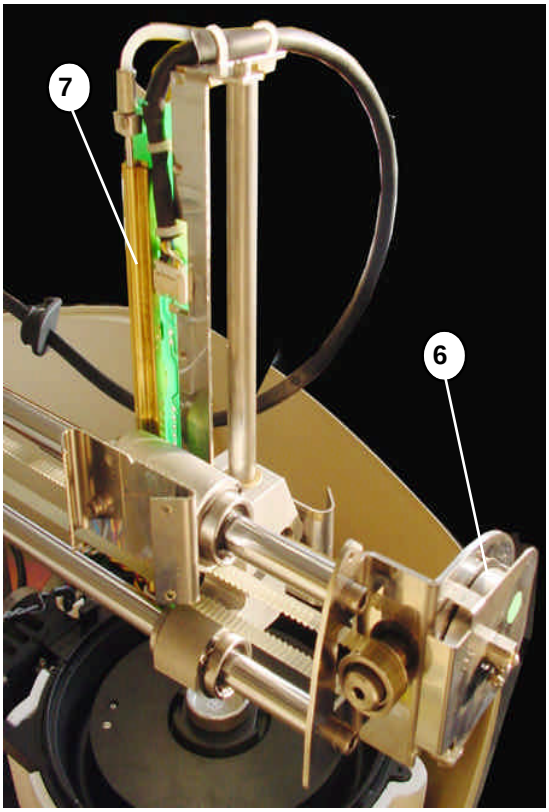

(1) Z GUIDE
(2) RACK
(3) Z MOTOR
(4) ENCODER
(5) TRANSMISSION AXIS
(6) RETURN SPRING
(7) THERMOSTATATION PIPE
(8) CONTROL PCB
(9) X CARRIAGE

The Z guide (1) supports the thermostatation pipe (7) and the control PCB (8) where the heating elements are located, together with the thermistor signal amplifier and level detection and the Z axis start photosensor. The rack (2) supports the Z guide (1) which crosses the Y carriage (9) on a bearing. The Z motor (3) is fastened to the X carriage (10) and is moved by a transmission axis (5) fitted with a pinion that acts on the rack. The return spring (6) acts on the transmission axis and prevents the needle from falling in the event of a power cut: The encoder (4), which detects any obstruction to the movement of the thermostated needle (9) is located on the same axis and on the part of the motor.

2.2.2. Dispensing system

The dispensing pump dispenses the preparations through the thermostated needle. The needle is washed internally and externally at the washing station. The racks tray makes it possible to position the samples to be analyzed and the required reagents. The level of the distilled water and waste containers is controlled by the analyzer by capacity.

2.2.2.1. Thermostated probe

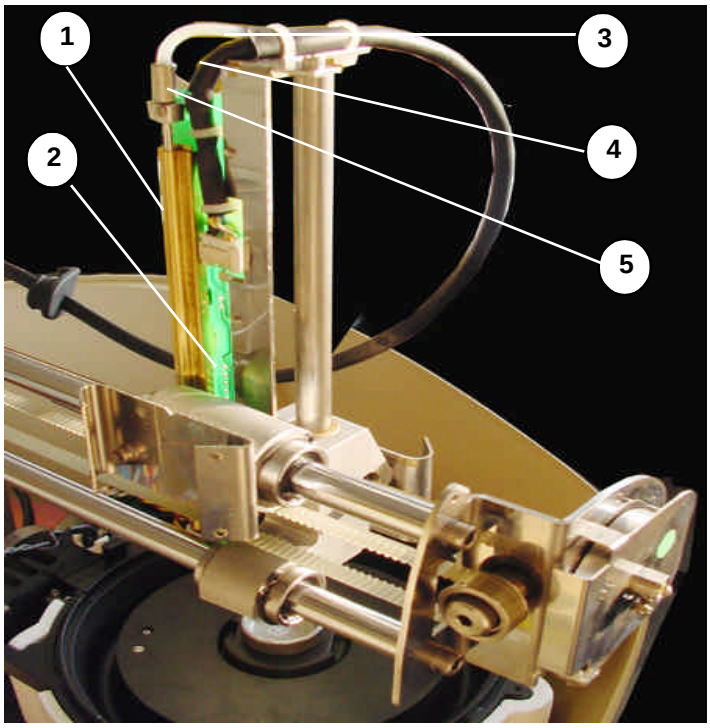

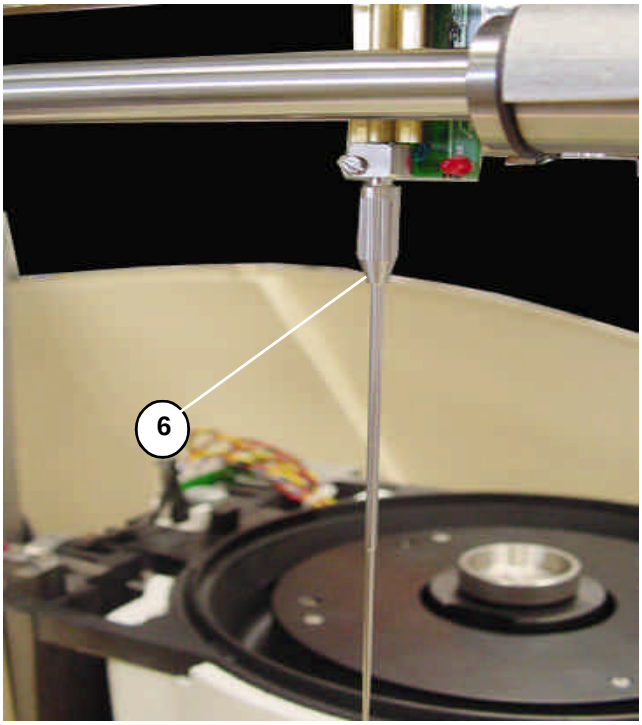

(1) THERMOSTATATION PIPE
(2) PCB
(3) TEFLON DISPENSING TUBE
(4) ELECTRICAL CONTROL HOSE
(5) FASTENING NUT
(6) REMOVABLE NEEDLE

The thermostatation pipe (1) preheats the reagent during dispensing. It is fitted with two connectors at each end. The removable needle (6) is connected to one and the Teflon dispensing pipe (3) is connected to the other, fixed by the fastening connector (5). The PCB (2) contains the thermostatation elements, the thermistor and associated circuits. The various thermistor and element action signals (3) pass through the hose (4).

2.2.2.2. Dispensing pump

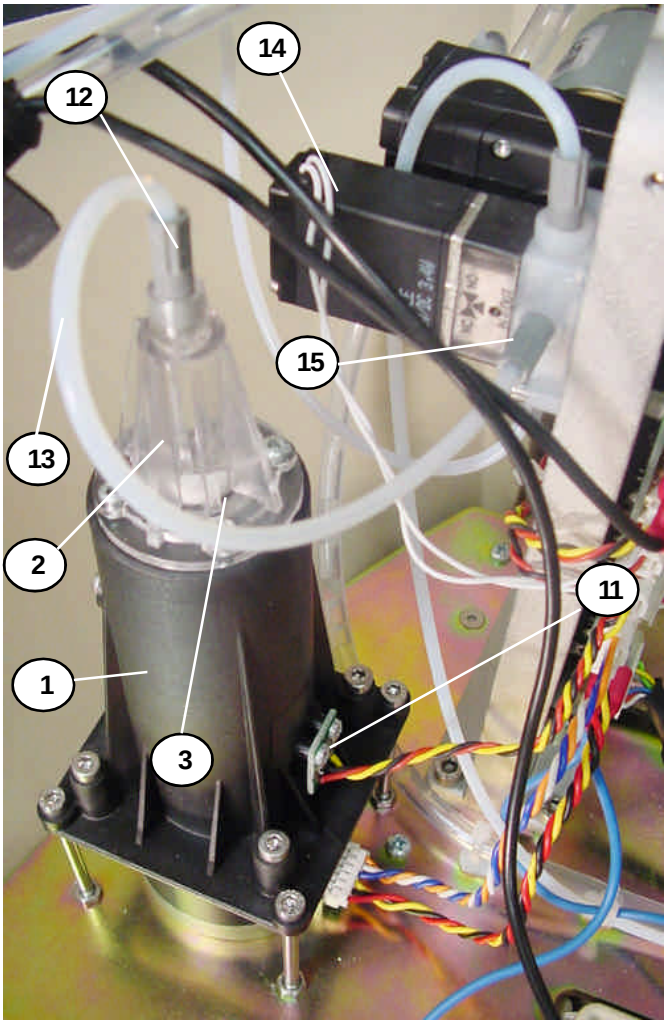

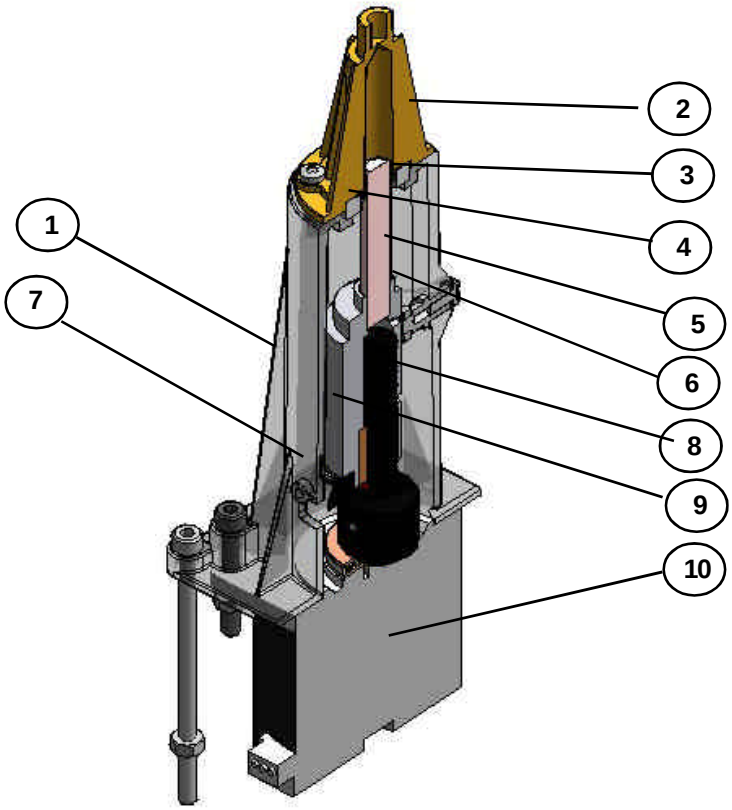

(1) BODY
(2) FLUIDIC CHAMBER
(3) SEAL
(4) SEAL SUPPORT
(5) CERAMIC PISTON
(6) PISTON SUPPORT
(7) START DETECTION BARRIER
(8) AXIAL BEARING
(9) ENDLESS SCREW
(10) MOTOR
(11) START PHOTOSENSOR
(12) PUMP NUT
(13) PUMP-ELECTROVALVE TEFLON TUBE
(14) 3-CHANNEL ELECTROVALVE
(15) ELECTROVALVE NUT

The plastic body (1) joins the different elements that make up the pump. The transparent methacrylate fluidic chamber (2) makes it possible to observe the flow of liquid through the pump. The support (4) fastens the seal (3) to the chamber. The ceramic piston (5) dispenses by displacing a certain volume of liquid in the chamber. The piston is adhered to the support (6), which moves alternatively by the rotation of the endless screw (9) fixed to the motor axle (10). The barrier (7), joined to the piston support, obstructs the photosensor (11) when the piston reaches its start position. The axial bearing (8) prevents any longitudinal displacement of the motor axle for greater precision in the dispensing operation. The 3-channel electrovalve (14) makes it possible to connect the pump chamber to the distilled water container or to the thermostated needle. The Teflon tube (13) connects the chamber to the electrovalve. It is connected to each of these elements by the nuts (13) and (15).

2.2.2.3. Tubes and containers

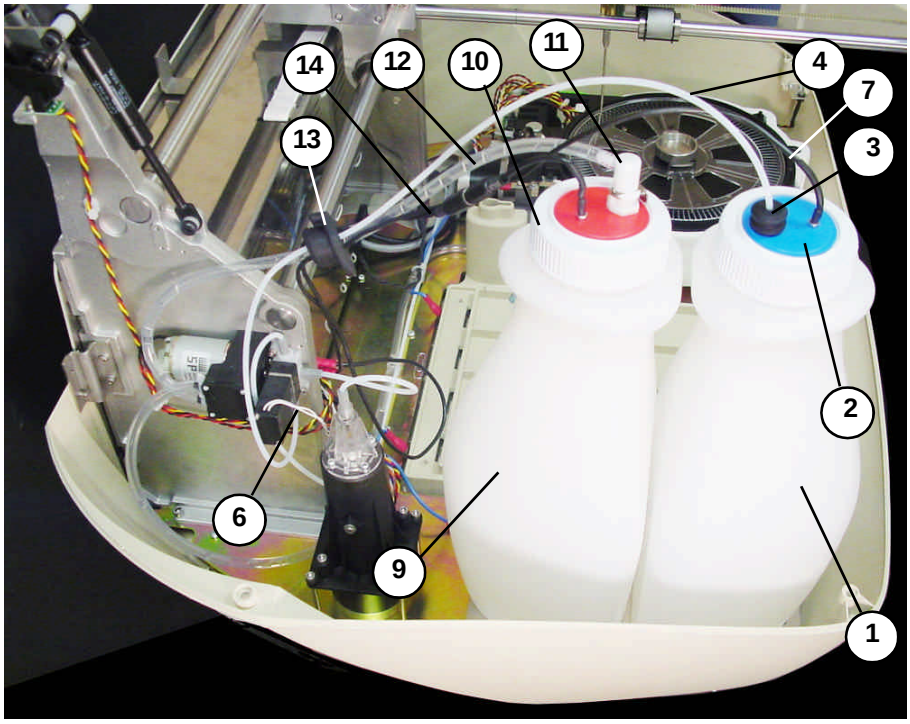

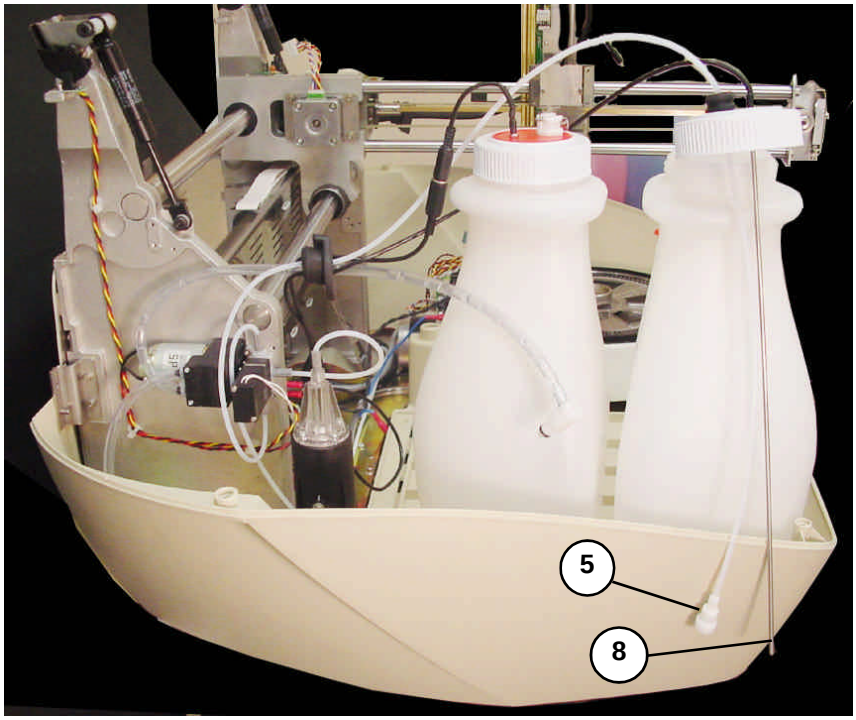

(1) WATER CONTAINER
(2) WATER CONTAINER LID
(3) WATER CONTAINER TUBES FASTENING
(4) WATER CONTAINER TEFLON TUBE
(5) TEFLON TUBE FILTER
(6) ELECTROVALVE NUT
(7) SYSTEM LIQUID LEVEL SENSOR CABLE
(8) LEVEL SENSOR
(9) WASTE CONTAINER

(10) WASTE CONTAINER LID
(11) FAST COUPLING NUT
(12) WASTE CONTAINER PVC TUBE
(13) GROMMET
(14) WASTE LEVEL SENSOR CABLE

The Teflon tube (4) connects the distilled water container (1) to the electrovalve of the dispensing pump. This tube is installed at the end of the filter container (5). It is connected to the electrovalve of the dispensing pump through the nut (6) The Teflon pipe passes through the rubber piece (3) in the lid (2) of the container, which fastens them in position. The PVC tube (12) connects the waste extraction membrane pump to the waste container (9). The waste container lid (19) has a fast coupling nut (11) with automatic drip-proof closing when disconnected. All the tubes pass into the interior of the analyzer through the rubber grommet (13).

2.2.2.4. Container level control sensors.

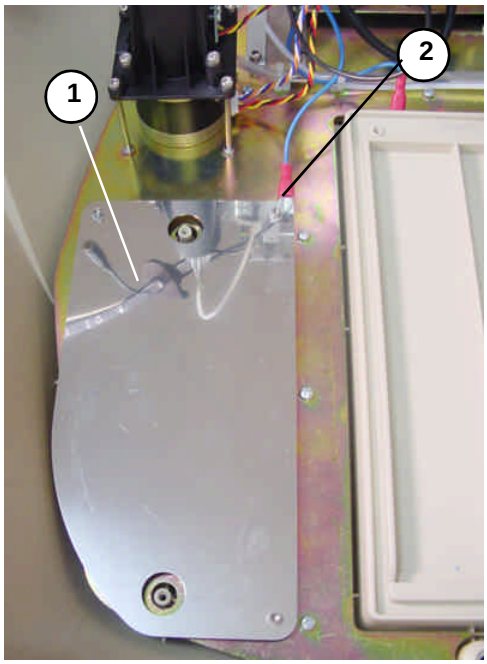

(1) LEVEL DETECTION SHEETING
(2) SIGNAL CONNECTOR

The analyzer has a capacitance system to control the level of the distilled water and waste containers. For this, there is an emission plane (1) under the bottles where a signal is injected through the connector (2). The base supporting the bottles is above this. They have 2 rods that collect the signal and indicate the presence or absence of liquid.

2.2.2.5. Racks tray with integrated washing station.

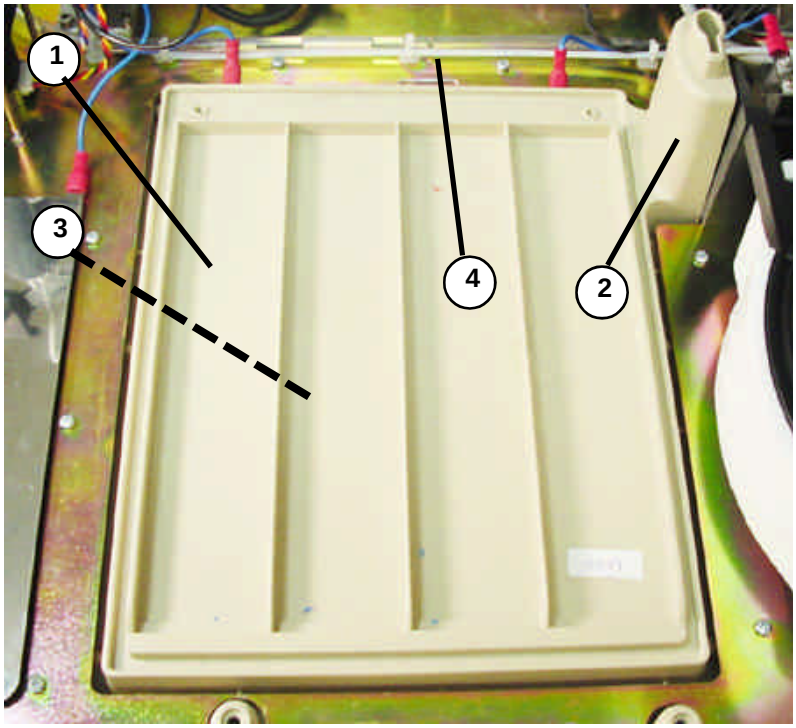

(1) TRAY
(2) WASHING STATION
(3) LEVEL DETECTION SHEETING
(4) WASTE PVC PIPE

The plastic injection tray (1) is part of the base of the instrument. The washing station (2) is installed on the right. The plate (3) detects the level of the dispensing needle. The PVC tube (7) connects the washing station drain to the waste extraction pump.

2.2.2.6. Washing pumps

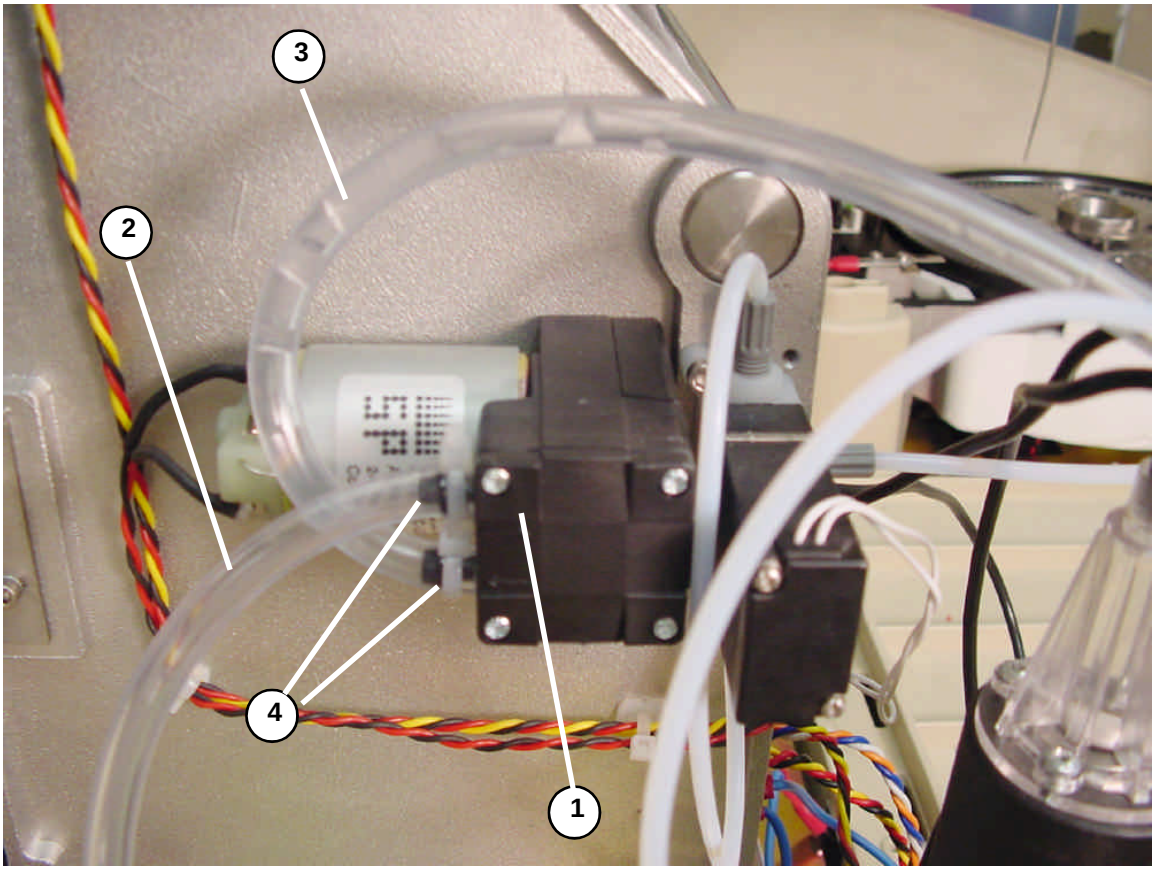

(1) MEMBRANE WASTE PUMP
(2) WASHING STATION-PUMP PVC TUBE
(3) WASTE BOTTLE-PUMP PVC TUBE
(4) SAFETY FLANGES

The needle washing system has a waste extraction pump (1). This is connected to the washing station by the PVC (2). The pump expels the waste through the pipe (4) into the waste bottle. The pipes are fastened by two safety flanges.

2.2.3. Reaction rotor with integrated optical system.

The reactions rotor is thermostated at 37ºC. The optical system, made up of a lighting system and a photometric system takes the readings directly on the rotor reaction wells. The lighting system has a halogen lamp, a filter drum for the selection of the wavelength form the appropriate beam of light. The photometric system contains a silicon photodiode and the corresponding electronics to obtain a digital value that is proportionate to the light intensity received.

2.2.3.1. Thermostated rotor and photometric system

(1) METHACRYLATE ROTOR

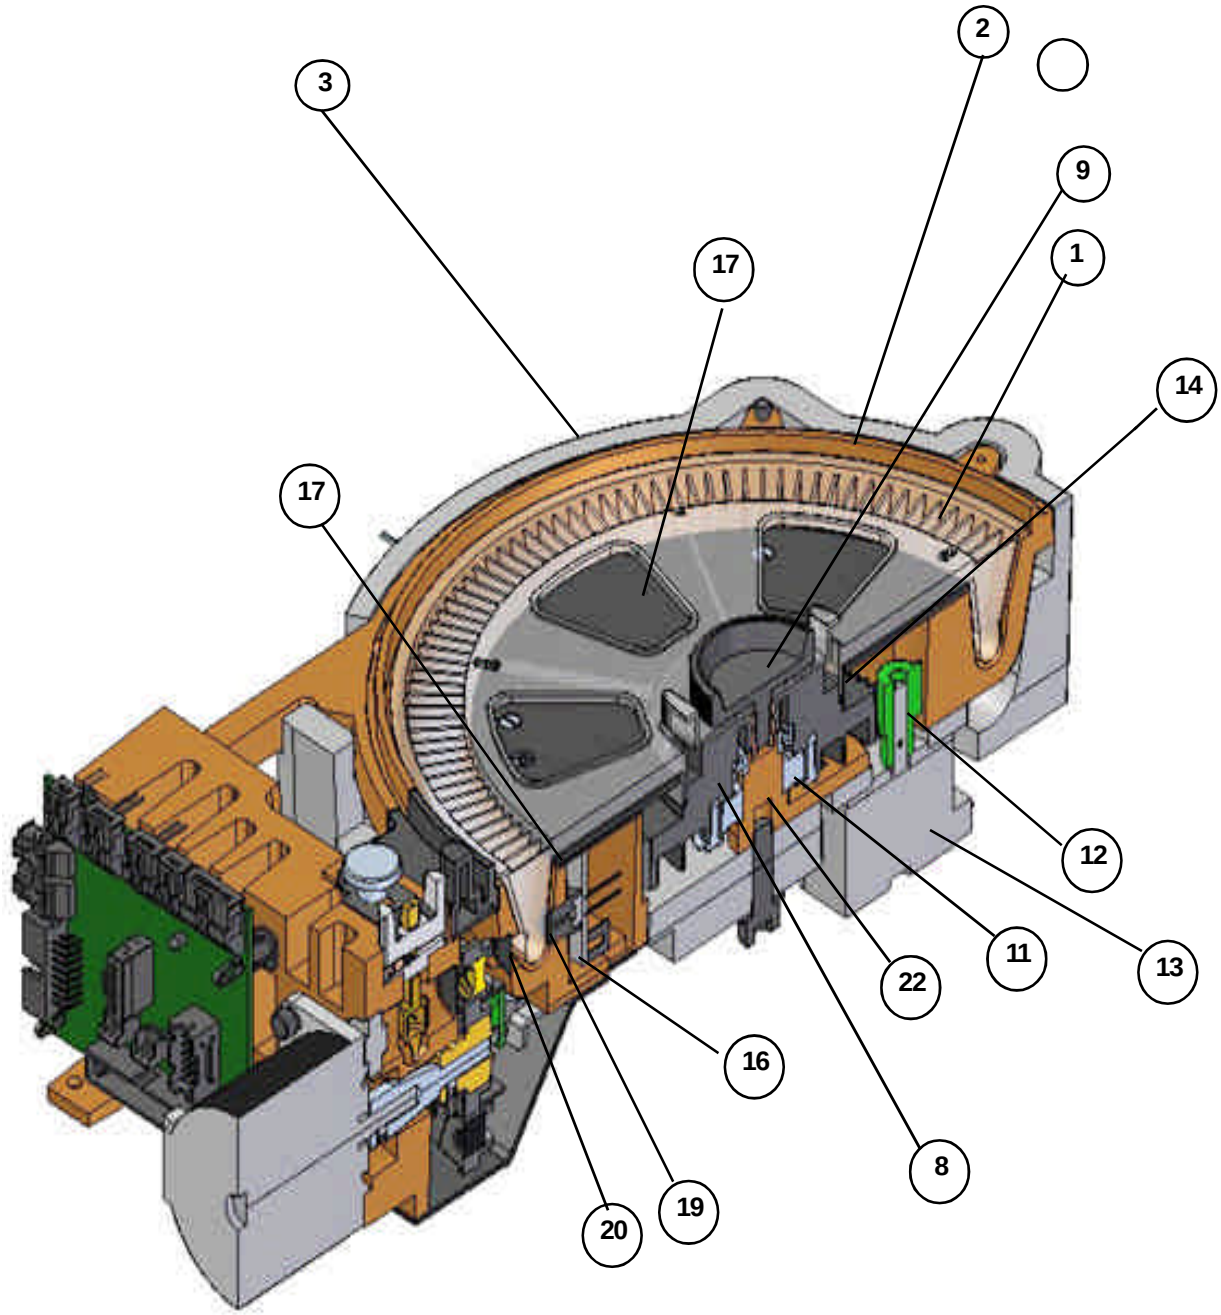

(2) HEATING CANAL
(3) THERMAL INSULATION OF THE HEATING CANAL
(4) PELTIER CELLS
(5) RADIATORS
(6) FANS
(7) TEMPERATURE PROBE
(8) ROTOR CENTRING UNIT
(9) ROTOR FASTENING SCREW
(10) START PHOTOSENSOR
(11) BEARINGS
(12) PINION
(13) MOTOR
(14) ROTOR CROWN
(15) MOTOR SEPARATOR

(16) PHOTOMETRIC SYSTEM BOARD
(17) ELECTRONIC BOARD SUPPORT COVER
(18) COVER
(19) PHOTODIODE GRILL CENTRING UNIT
(20) ROTOR GRILL
(21) COVER DETECTOR
(22) ROTOR AXLE

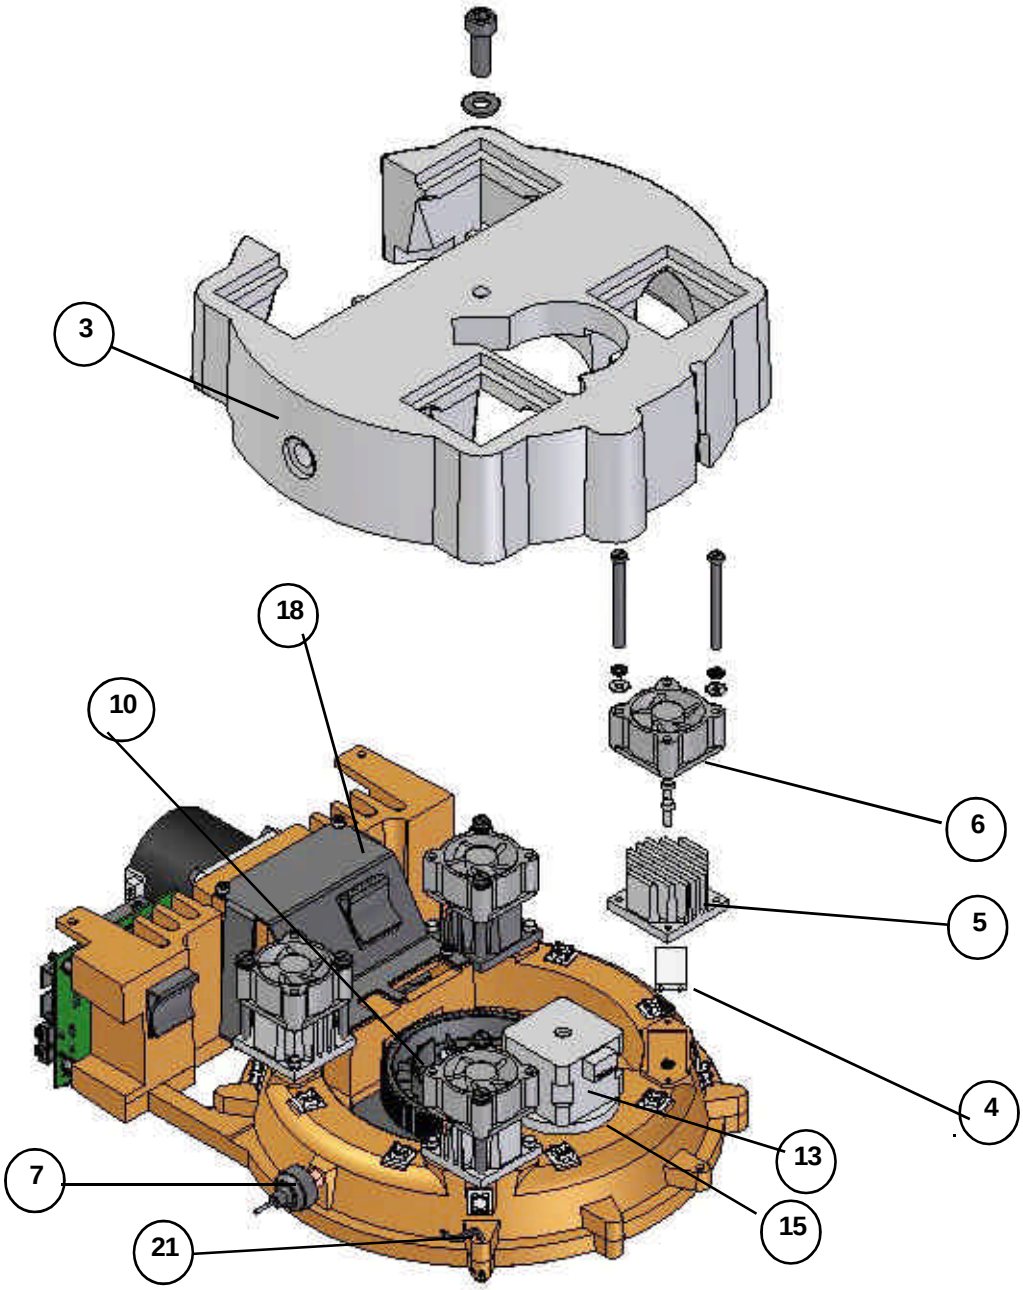

The dispensing system dispenses the reagents and the samples in the methacrylate rotor (1). The optical system measures the absorbance directly on the rotor wells. The aluminium heating canal (2) surrounds the rotor and keeps it at 37ºC. The canal is thermally insulated from the exterior by means of the moulded expanded polystyrene insulation (3). The Peltier cells (4), with their respective radiators (5) and fans, act on the canal to control the temperature. The sensor used to control the temperature is the probe (7). The methacrylate rotor is fastened to its centring unit (8) by means of the screw (9). The centring unit is fixed to the heating canal through the axis (22), which is fitted on bearings (11). The barrier obstructing the photosensor (10) when the rotor reaches its start position forms part of the centring

unit (8). The centring unit also acts as gearing. The pinion (12), fixed to the motor (13), acts through the crown (14), which also acts as a centring unit. The separator (15) does not allow the motor temperature to reach the heating canal. The electronic board of the photometric system (16) is housed in a cavity in the heating canal. The upper cover of this cavity (17) supports the electronic board. The seal (18) keeps the cavity hermetically closed in the case of possible liquid spillage. The housing of the filter drum is closed at the bottom by the cover (18). The part (19) centres the photodiode with regard to the lighting system and also acts as a grill to prevent the incidence of unwanted light. The grill (20) limits the light hitting the reactions rotor. The detector (21) tells the analyzer if the rotor cover is in position or not.

2.2.3.2. Lighting system

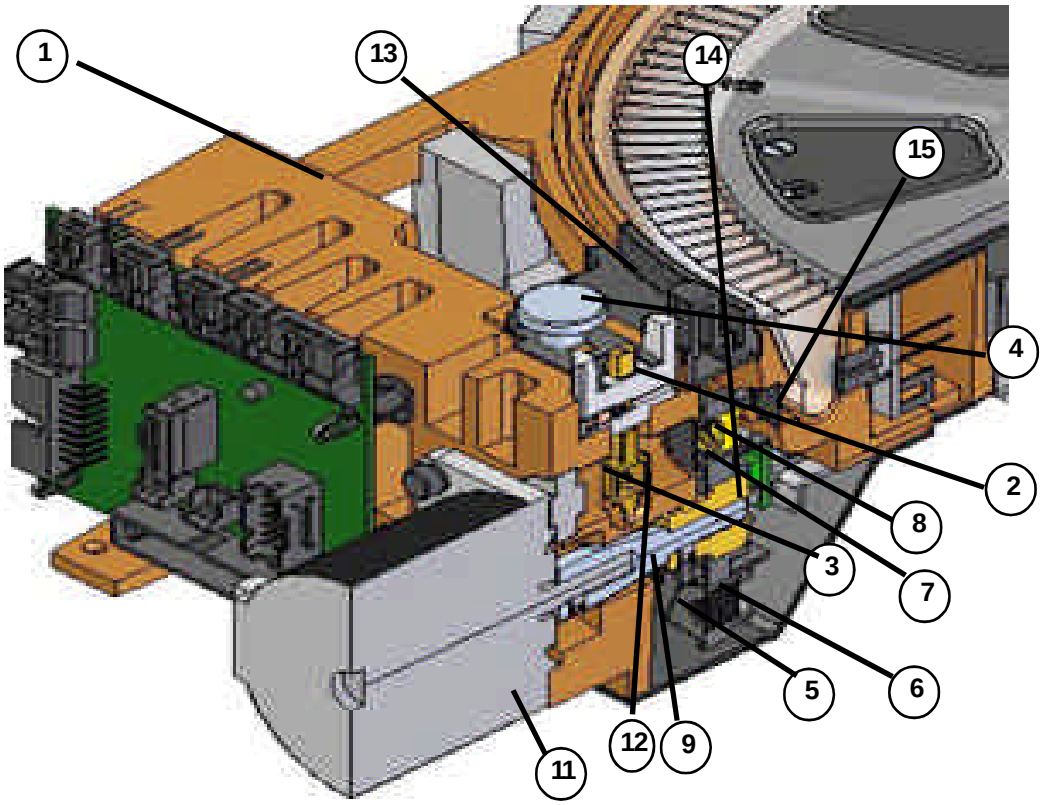

(1) BODY
(2) LAMP HOLDER
(3) HALOGEN LAMP
(4) LAMP HOLDER FASTENING
(5) FILTER DRUM
(6) FILTER HOLDER
(7) FILTER HOLDER NUT
(8) MATCHED INTERFERENTIAL FILTERS
(9) DRUM AXLE
(10) START PHOTOSENSOR
(11) MOTOR
(12) DIAPHRAGM
(13) FILTER DRUM WINDOW COVER
(14) BEARING
(15) APERTURE

The aluminium body (1) is the structure that supports all the elements of the lighting system. The lamp holder (2), fastened to the body by means of the fastening system (4), keeps the halogen lamp (3) in position without the need for adjustments. The filter drum (5) has 10 positions for optical filters. Position 0 must always be taken up by a covered filter. The other positions can be taken up by an interferential filter (8) or by other covered filters. No position in the drum must be left unoccupied. Each filter is fitted on a filter holder (6) and fastened to it by the nut (7). The filter holders can be dismounted from the drum by simply pulling on them. The cover (13) allows easy access to the filter drum. The filter

drum is fastened to the axle (9). This axle can be turned by the direct action of the motor (11). Its end is guided by the bearing (14). The photosensor (10) indicates the start position of the drum. The light from the lamp, limited by the diaphragm (12). The light passes through the filter drum, which selects the desired wavelength, and through the aperture(15), which adapt the form of the light beam to the geometry of the rotor wells.

2.2.4. Electronics cover

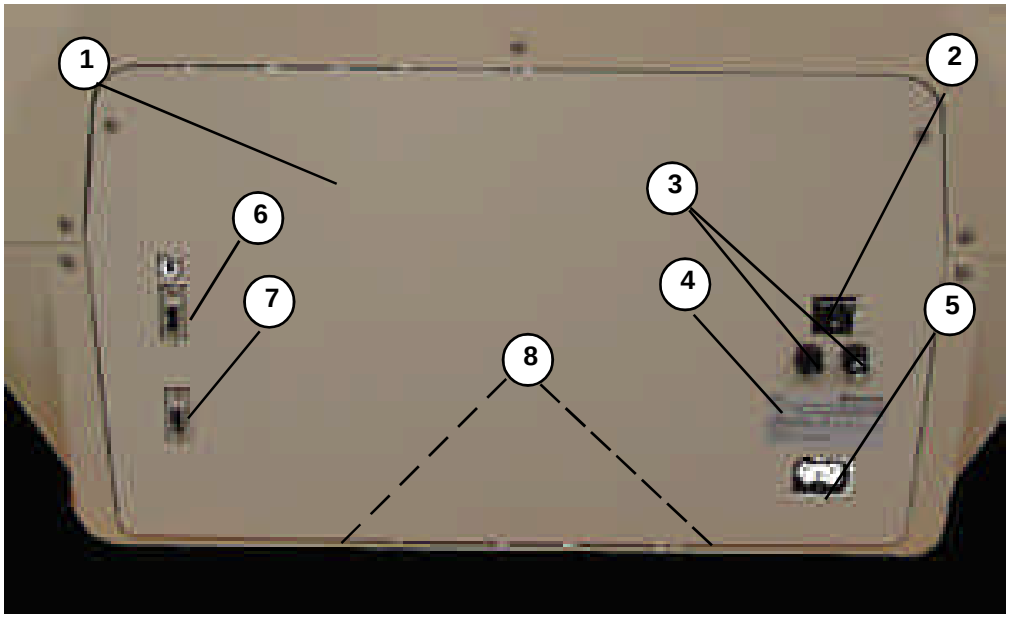

(1) BACK COVER OF THE ELECTRONICS
(2) MAINS SWITCH
(3) FUSE HOLDER
(4) ID LABEL
(5) NETWORK CONNECTOR
(6) COM1 CONNECTOR
(7) COM2 CONNECTOR
(8) HINGES

The metal cover (1) supports the mains switch (2) and the fuse holders (3), as well as the identification label (4). The COM1 and COM2 connectors (6, 7) and the mains connector (5) are fastened to the electronics box. The cover(1) opens on 2 hinges (7).

2.2.5. Main cover hinges

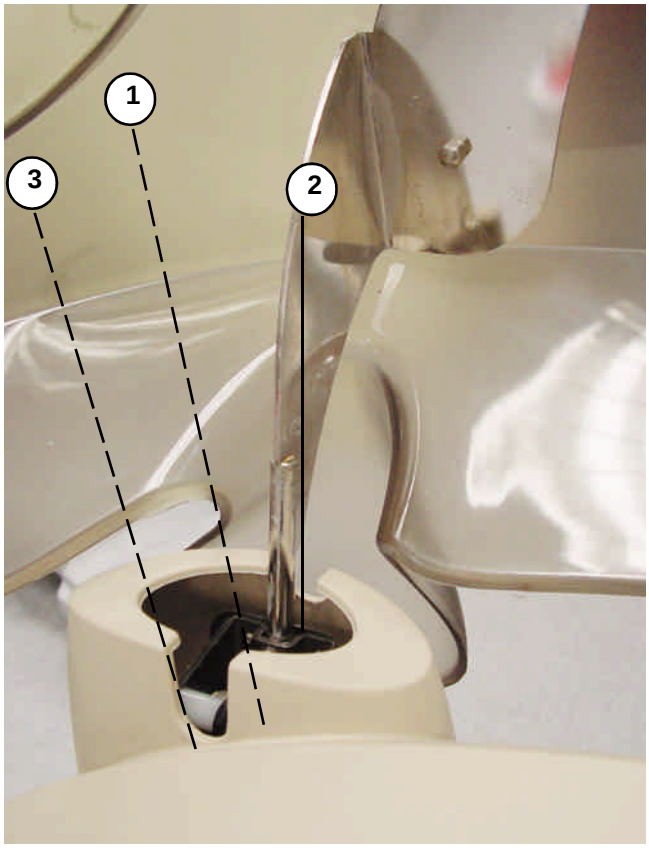

(1) HYDRO-PNEUMATIC SPRING
(2) ARTICULATED STEEL STRUCTURE
(3) COVER OPEN PHOTOSENSOR (on right-hand hinge only)

The two hinges enabling the raising of the main cover of the analyzer consist of an articulated steel structure (2) operated by a hydro-pneumatic spring (1). The right-hand hinge includes a photosensor (3) to detect whether or not the cover of the analyzer is open or closed.

2.2.6. Base

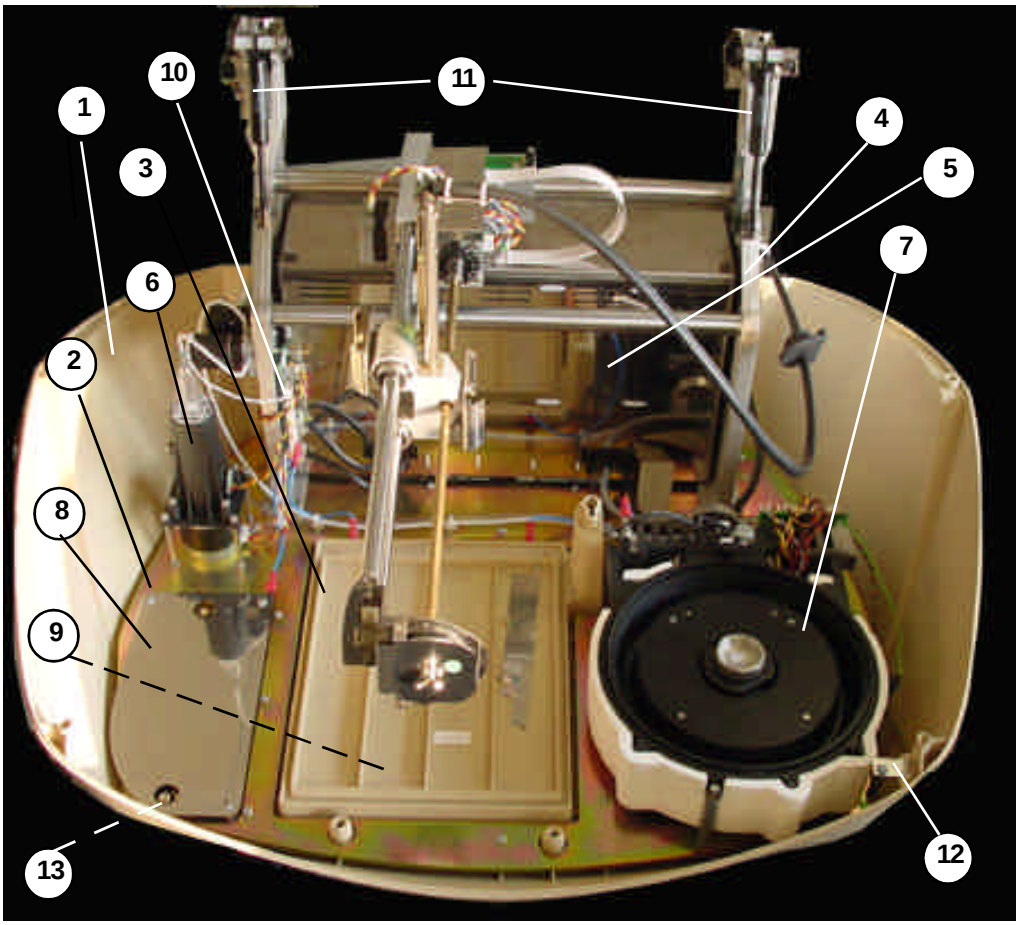

(1) LOWER PLASTIC CASING
(2) BASE
(3) WASHING STATION AND RACK TRAY
(4) ARM UNIT
(5) ELECTRONICS BOX
(6) DISPENSING PUMP
(7) REACTION ROTOR AND INTEGRATED OPTICAL SYSTEM
(8) BOTTLE LEVEL DETECTION PLATE
(9) LEVEL DETECTION PLATE
(10) PUMP AND MICROPROCESSOR INTERCONNECTION BOARD
(11) MAIN COVER HINGES
(12) FRONT INDICATOR
(13) ADJUSTABLE LEG

The base (2) on which all the elements of the analyser are fixed is fastened directly to the lower plastic casing. The rack tray and washing station form part of the base. The instrument stands on 4 rubber legs . The front right leg (13) is adjustable in height to adapt the instrument to the work surface.

2.2.7. Casings

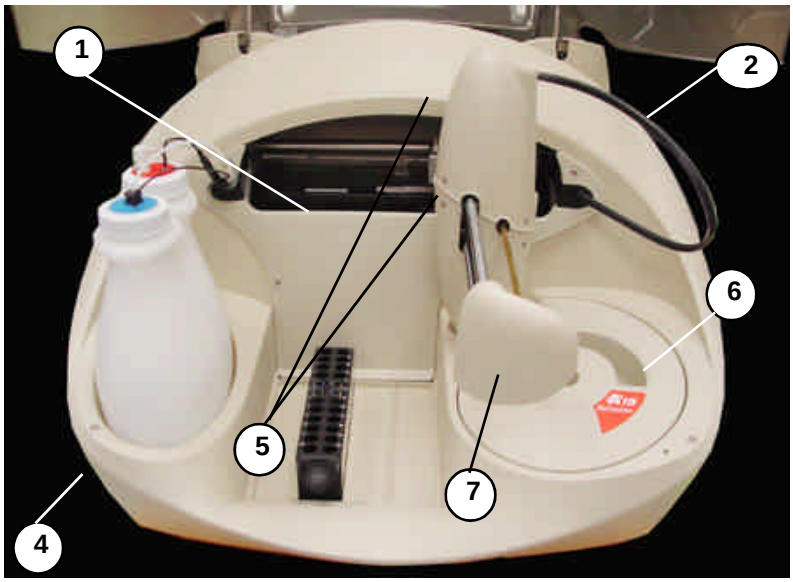

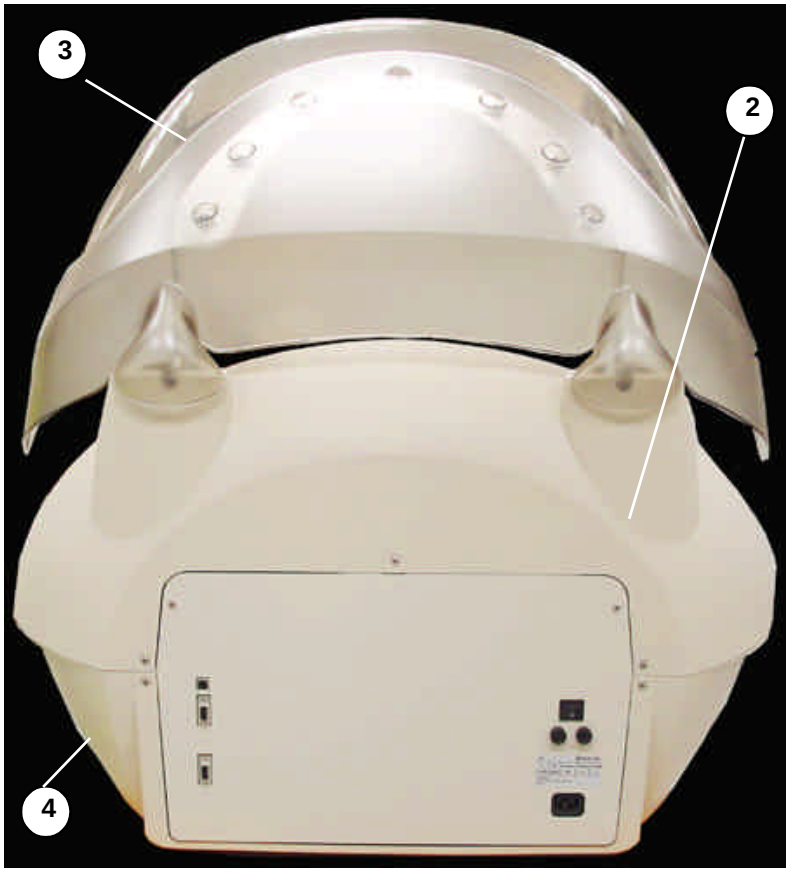

(1) FRONT CASING
(2) UPPER CASING
(3) MAIN COVER
(4) LOWER CASING
(5) ARM HOUSING
(6) ROTOR COVER
(7) RETURN SPRING COVER

The front casing (1) is fastened to the upper casing (2) and the upper casing is fastened to the lower casing (4). The top cover (3) is transparent and lets users see the analyser in operation with the cover closed.

3. ELECTRONIC SYSTEM

1. Description of the electronics of the A15 analyzer.
2. CPU Board (CIIM00026)
3. Power supply board and source (SP150 & CIIM00015)
4. Needle Board (CIIM00017)
5. Photometry Board (CIIM00027)
6. XYZ carriage interconnection board (CIIM00018)
7. Rotor interconnection board (CIIM00029)
8. Fluid interconnection board (CIIM00028)
9. Communications Board (CIIM00036)
10. Interconnection between boards

Description of the electronics of the A15 analyzer.

The electronics of the analyzer are made up of different boards located at different points in the analyzer and dedicated to specific functions. Its different location corresponds to functionality and performance criteria for the functioning of the analyzer.

There are 8 different boards, which correspond to:

CPU Board (CIIM00026)
Power supply board and source (SP150 & CIIM00015)
Needle Board (CIIM00017)
Photometry Board (CIIM00027)
XYZ carriage interconnection board (CIIM00018)
Rotor interconnection board (CIIM00029)
Fluid interconnection board (CIIM00028)
Communications Board (CIIM00036)

3.1 CPU Board (CIIM00026)

This is the brain of the machine, containing the microprocessor (H8/3003), responsible for controlling all the elements of the machine. The board has different data storage systems using either static RAM (U1 and U47), FLASH memory (U10) or EPROM (U9). The slot associated with the EPROM is used to check the functionality of the board and the recording of the MONITOR program in the production phases of the analyzer. The other two memories are associated with the normal functioning of the analyzer. The FLASH memory holds the application itself as well as different databases related to factory settings, adjustments, state of the rotor and possible extensions to the application.

The U21 device also exists on the board. This is a logical programmable device (FPGA) dedicated to the control of motors, mapped in register memory associated with end-of-run control, electrovalves, level sensing and control of the photometry-associated board (CIIM00027).

The motor control acts directly on the drivers corresponding to each of the analyzer's axes (U28,U29,U30,U24,U25,U27) to act on the motor. The driver comprises the L6228 integrated circuit. The regulation of the current of each axis can be configured by means of a DAC that sets the current set point independently (U26).

The action on the thermostatation systems of the rotor is carried out through H-shaped bridges based on MOS technology (U45) and controlled directly from the microprocessor. The action on the needle thermostatation system is through the Q4 transistor.

Connector	Function	Pins
J1	Not available	
J2	Connection to communications board (CIIM00036)	1 - V DC 2 - GND 3 - Tx0 4 - GND 5 - Rx0 6 - GND 7 - GND 8 - Tx1 9 - GND 10 - Rx1
J4	Connection to XYZ interconnection board (home and encoder signals)	1 - V DC 2 - GND 3 - Needle encoder 4 - Home motor Y 5 - Home motor X 6 - GND
J5	Connection to XYZ interconnection board (motor signals)	1 - coil 2 motor X 2 - coil 2 motor X 3 - coil 1 motor Y 4 - coil 1 motor X 5 - coil 1 motor Y 6 - coil 1 motor X 7 - coil 2 motor Y 8 - coil 2 motor Z 9 - coil 2 motor Y 10 - coil 2 motor Z 11 - coil 1 motor Z 12 - coil 1 motor Z
J6	Connection to interconnection board Rotor (home motor signals and photometry board control signals)	1 - 12 V 2 - GND 3 - DVALID 4 - DCLK 5 - DOUT 6 - DXMIT 7 - RANGE2 8 - RANGE1 9 - RANGE0 10 - TEST 11 - CONV 12 - GND 13 - CLKAD 14 - GND 15 - GND 16 - V DC 17 - V DC 18 - Rotor cover 19 - GND 20 - Rotor thermistor 21 - Home motor filter drum 22 - GND 23 - Home motor rotor 24 - Front red LED 25 - Front green LED

Connector	Function	Pins
J7	Connection to rotor interconnection board (motor and Peltier signals)	1 - coil 2 motor filters 2 - coil 2 motor filters 3 - coil 1 motor filters 4 - coil 1 rotor motor 5 - coil 1 motor filters 6 - coil 1 rotor motor 7 - Peltier 8 - coil 2 rotor motor 9 - Peltier 10 - coil 2 rotor motor 11 - V(24 V) 12 - Peltier fans
J8	Connection to interconnection board fluids (electrically operated valve and pump signals)	1 - V(24 V) 2 - Waste pump 3 - V(24 V) 4 - Electrically operated valve 5 - coil 1 ceramic pump 6 - coil 1 ceramic pump 7 - coil 2 ceramic pump 8 - coil 2 ceramic pump
J9	Connection to interconnection board fluids (ceramic pump home and level sensor signals)	1 - Waste bottle sensor input 2 - System liquid sensor input 3 - Bottle detection signal 4 - Rack level detection signal 5 - Ceramic pump home 6 - V DC 7 - GND 8 - Instrument cover detection
J10	Connection to needle board	1 - V (12 V) 2 - GND 3 - Home motor Z 4 - Needle thermistor 5 - Rack level detection signal 6 - V (24 V) 7 - Needle thermostat elements 8 - NC
J11	Connection to supply board	1 - V (12 V) 2 - GND 3 - V (24 V) 4 - V DC 5 - Fan control 6 - Lamp control

Analogical circuitry:
The waste and system liquid sensors function through U6, U5 and U4, which generate and detect the signal responsible for detecting the waste and system liquid. These signals are sent and received through the fluid interconnection board (connected to the CPU board by J9). The rack level detection is carried out in a similar way through U7, U8 and U2. The signal injected to the base of the bottles goes to the fluid interconnection board through J9 and is collected after it has been amplified by J10 (connection with the needle board). There is also a circuit for conditioning the signal of the thermistor associated with the thermostatation of the rotor that is made up of the U1 and U2 circuits. The thermistor is connected to the rotor interconnection board, which is connected to the CPU board.
TP1 - Waste pump control signal
TP2 - Electrovalve control signal
TP3 - Rotor thermistor signal
TP4 - RESET
TP5 - WATCHDOG
TP6 - LSO_BOT bottle detection signal
TP7 - Bottle signal
TP8 - Needle detection signal
TP9 - LSO needle detection signal
TP10 - Attenuated LSO needle detection signal
TP11 - IN1 Needle Peltier Driver
TP12 - Needle resistance driver
TP19 - ASL
TP20 - HWR_L
TP21 - LWR_L
TP22 - WE_L
TP24 - CS_FPGA_L
TP25 - DVALID (photometry)
TP26 - 12 Volts analogical
TP27 - IN2 Needle Peltier Driver
TP28 - EF Needle Peltier Driver
TP30 - DOUT (photometry)
TP33 - RANGE (photometry)
TP34 - CLKAD (photometry)
TP35 - Conditioned thermistor signal
TP38 - DXMIT (photometry)
TP39 - Analogical GND
TP40 - Power GND
TP41 - Power GND
TP42 - Power GND
TP43 - Digital GND
TP44 - Digital GND
TP45 - Digital GND

LIST OF LED DIODES

DL1 - Electrovalve driver
DL2 - Waste pump driver
DL3 - PELTIER heating
DL8 - PELTIER cooling
DL4 - Needle resistance driver

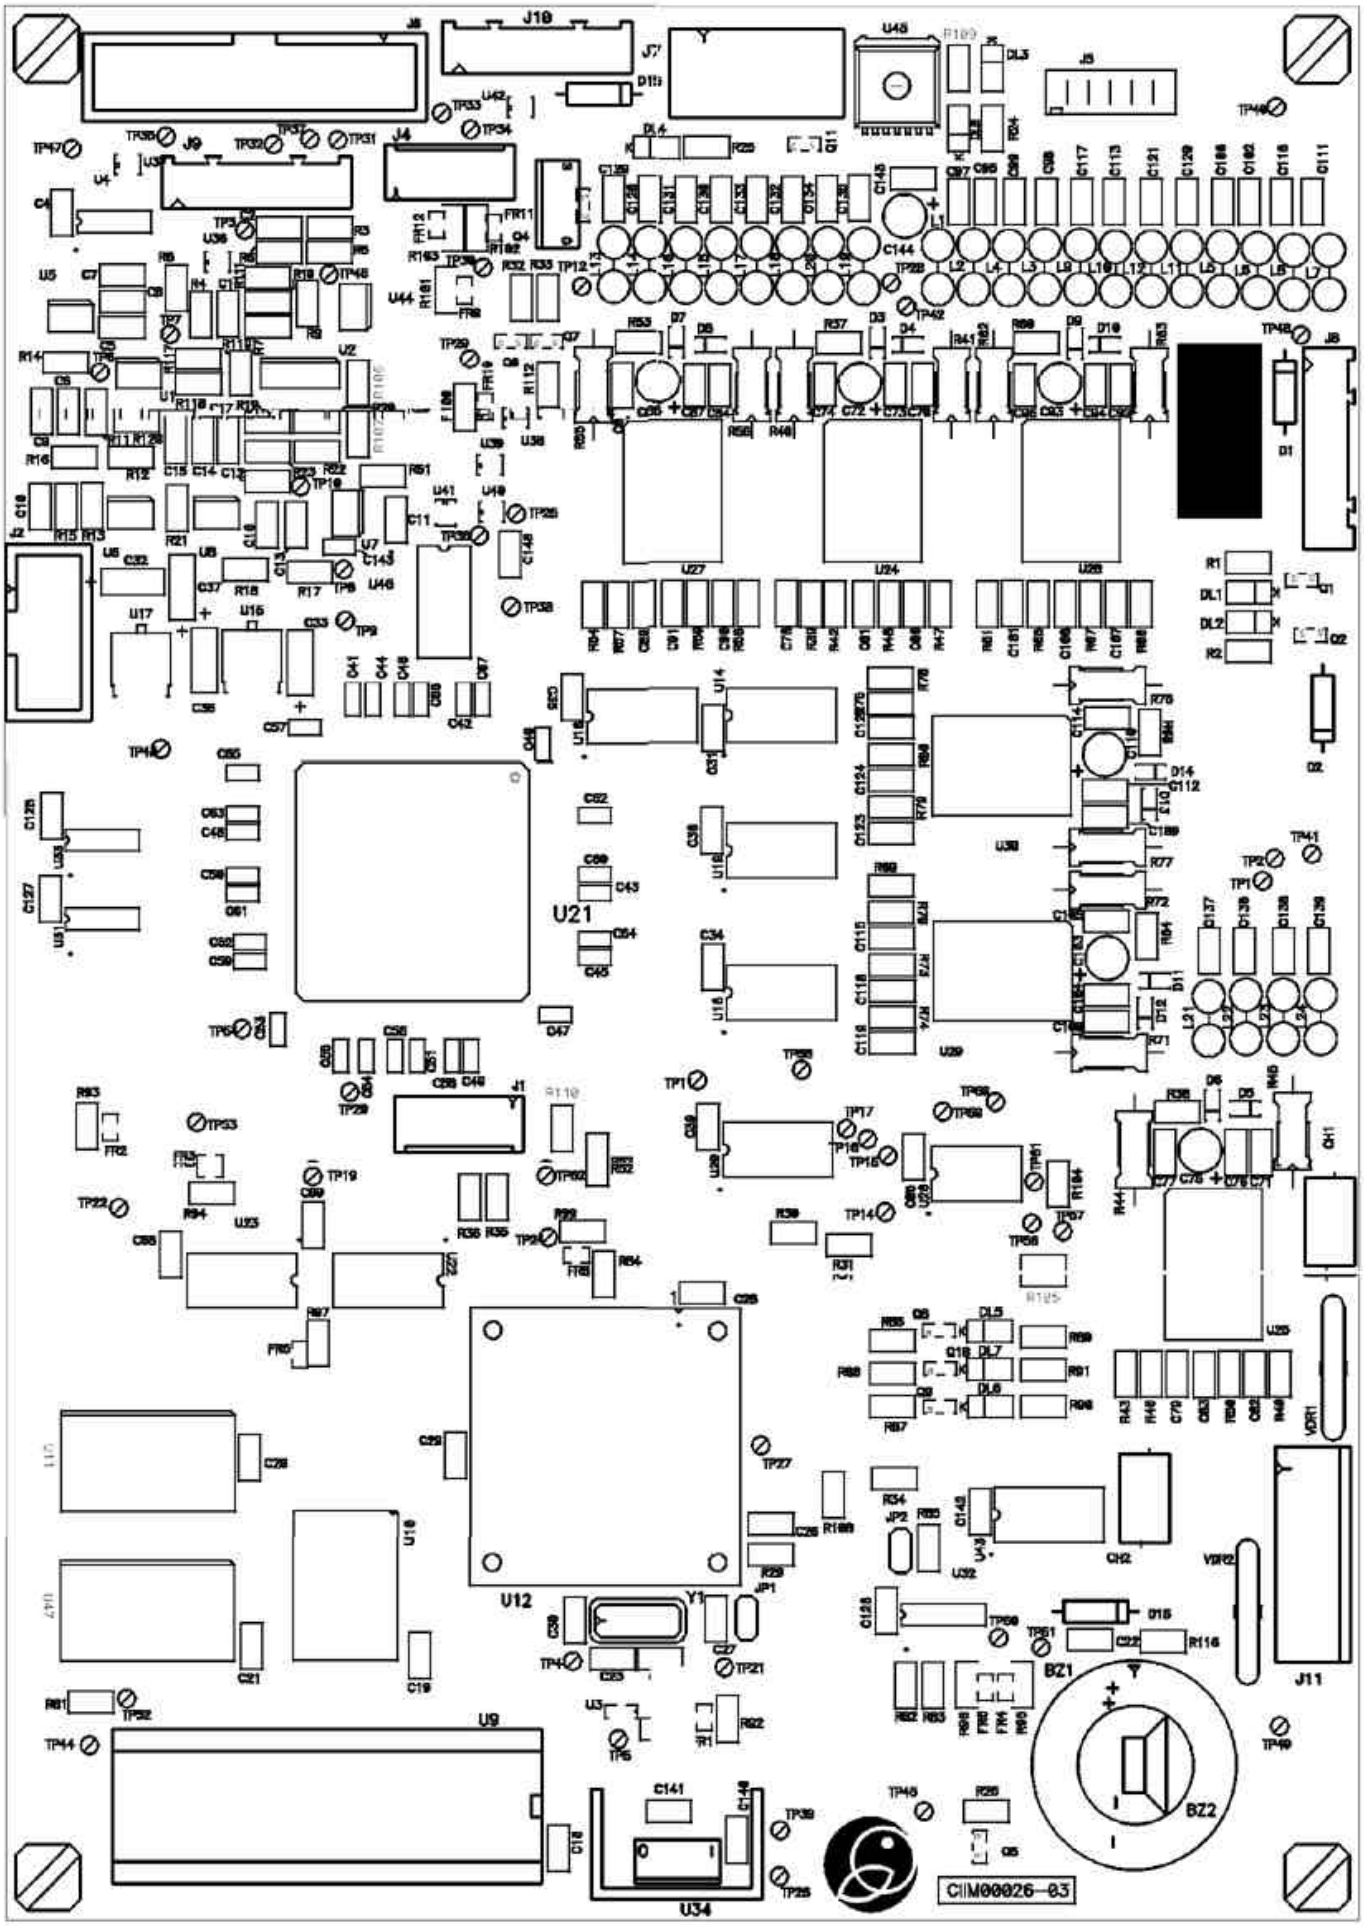
U21
U12
U34
BZ1
BZ2
J11
CIM00026-03

3.2 Power Supply Board (CIIM00015)

This is made up of 2 different switched regulators and 1 voltage line that enable distribution of the power supply in accordance with the requirement of each subsystem.

Connector	Function	Pins
J1	24 V input	1 - 24V 3 - (GND)
J2	Output voltage of 6 V for lamp supply	1 - 12 V 3 - GND
J3	Output voltage of 24 V, 12V, 5 V and fan and lamp control input	1 - 36V 2 - GND 3 - 12V 4 - 5V 5 - ENABLE LAMP 6 - ENABLE FAN
J4, J5	Fan output voltage of 24 V	1 - 24V 2 - GND

TP1 - Lamp voltage from 5.75 V <6V
TP2 - 12V analogicals
TP3 - 5V digital

List of LED diodes:

D4 - Indicates 5V activated
D2 - Indicates 12V lamp activated
D3 - Indicates 12V analogicals activated

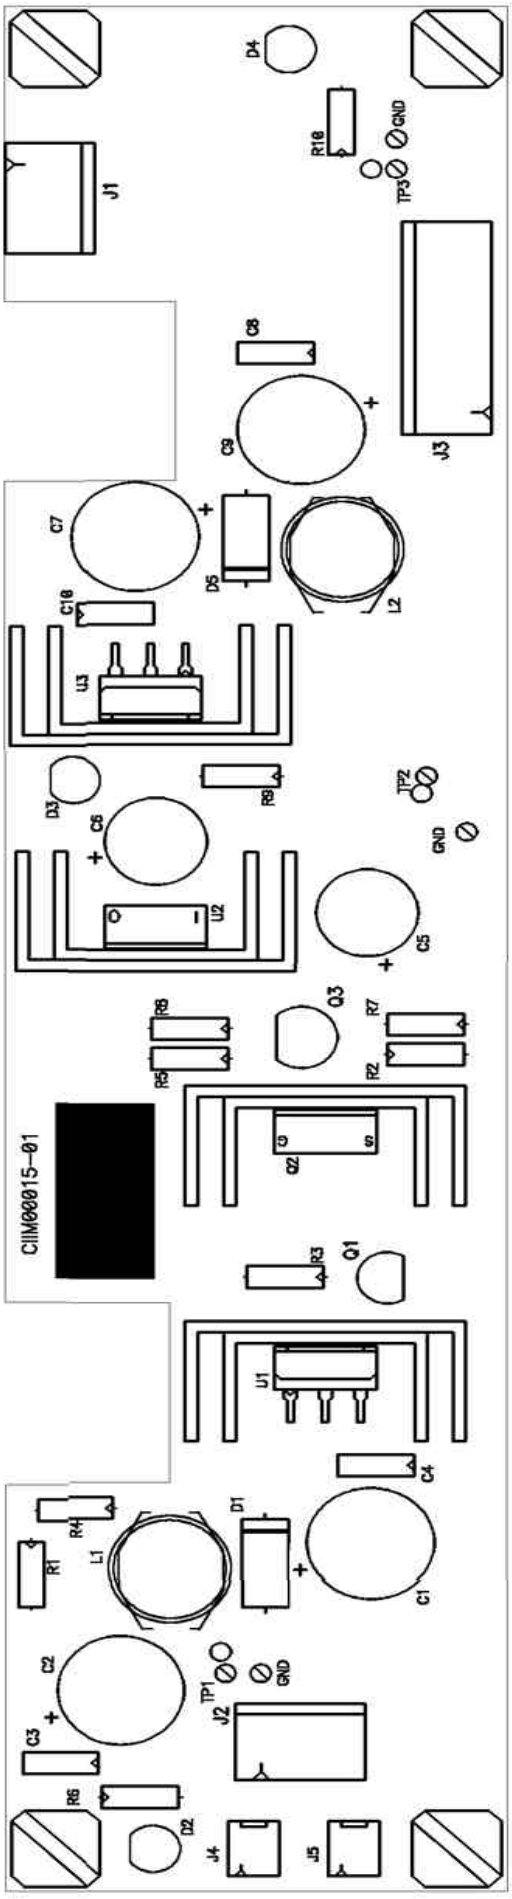
D4
R16
GND
TP3
J1
J3
C8
C9
C7
D5
L2
C10
U3
D3
R9
TP2
GND
C6
U2
C5
R8
Q3
R7
R5
R2
Q2
CIIM00015-01
R3
Q1
U1
C4
D1
R4
R1
L1
C1
C2
TP1
GND
J2
C3
R6
D2
J4
J5

3.3 Needle Board (CIIM00017)

This board conditions the thermistor signal associated with the thermostatation of the needle, the preamplification of the level detection signal and the Z home. It receives, from the needle unit, the thermostatation elements, the thermistor and the level signal detected by the needle itself.

The cables that join this board with the CIIM00026-01 board come from this needle.

Connector	Function	Pins
J1	CPU board connection (CIIM0026)	1 - GND POWER 2 - 12V analogical 3 - level sensor 4 - Home Z 5 - GND POWER 6 - Thermistor 7 - EARTH 8 - GND POWER 9,10 - Thermo elements.

TP1 - Needle signal
TP2 - Output preamplifier needle signal
TP3 - Output amplifier thermistor signal
TP4 - Thermistor
12V - 12V voltage
5V - Voltage 5V
AGND - GND

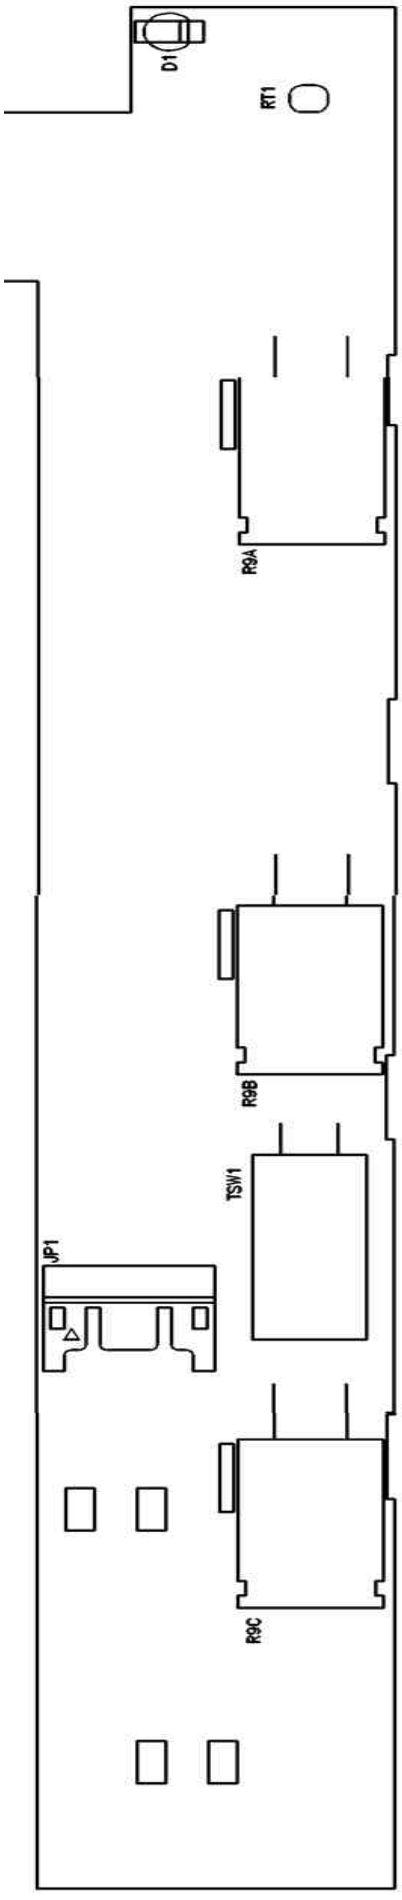
D1
RT1
R9A
R9B
TSW1
JP1
R9C

3.4 Photometry Board (CIIM00027)

This board also has the heart of the absorbance measuring system for the samples to be analyzed. It is made up of a photosensor and an associated analogical-digital conversion circuitry (DDC112).

Connector	Function	Pins
J3	Photometric board connection CIIM00029)	1 - 12 V 2 - GND 3 - DVALID 4 - DCLK 5 - DOUT 6 - DXMIT 7 - RANGE2 8 - RANGE1 9 - RANGE0 10 - TEST 11 - CONV 12 - GND 13 - CLKAD 14 - GND 15 - GND 16 - V DC

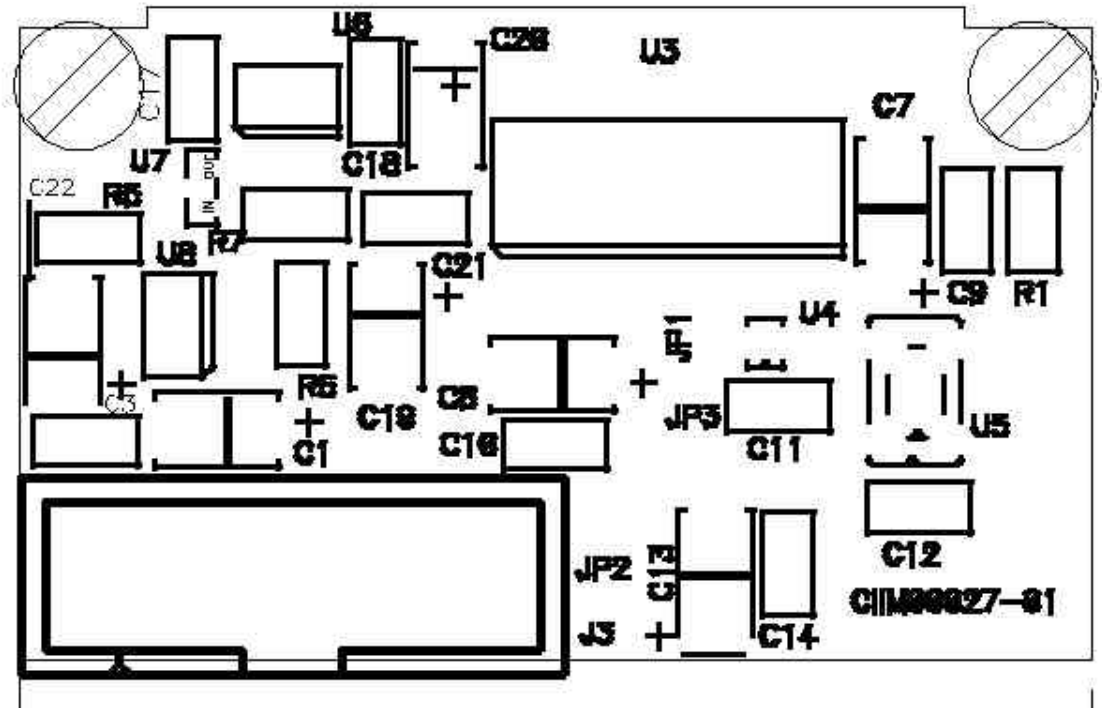

JP1 - soldering bridge - Solder only if the local oscillator and the U4 and U5 scales, respectively, are not present.
JP2 - soldering bridge - as per JP1
JP3 - soldering bridge - joins together the analogical and digital frames

3.5 XYZ Interconnection Board (CIIM00018)

This board interconnects the CP1 board with the X carriage. It distributes the X and Y motor signals and transmits the home signals of the X and Y movements. It also sends the encoder signal to the CPU board.

Connector	Function	Pins
J1	Connection motor X	
J2	Connection motor Y	
J3	Connection motor Z	
J4	CPU board connection (CIIM00026)	1 - coil 2 motor Y 2 - V DC 3 - coil 2 motor Y 4 - GND 5 - coil 1 motor Y 6 - encoder 7 - coil 1 motor Y 8 - home motor X 9 - coil 2 motor Y 10 - home motor X 11 - coil 2 motor Z 12 - GND
J5	CPU board connection (CIIM00026)	1 - coil 2 motor X 2 - coil 2 motor X 3 - coil 1 motor X 4 - coil 2 motor Z 5 - coil 2 motor Z 6 - coil 1 motor Z

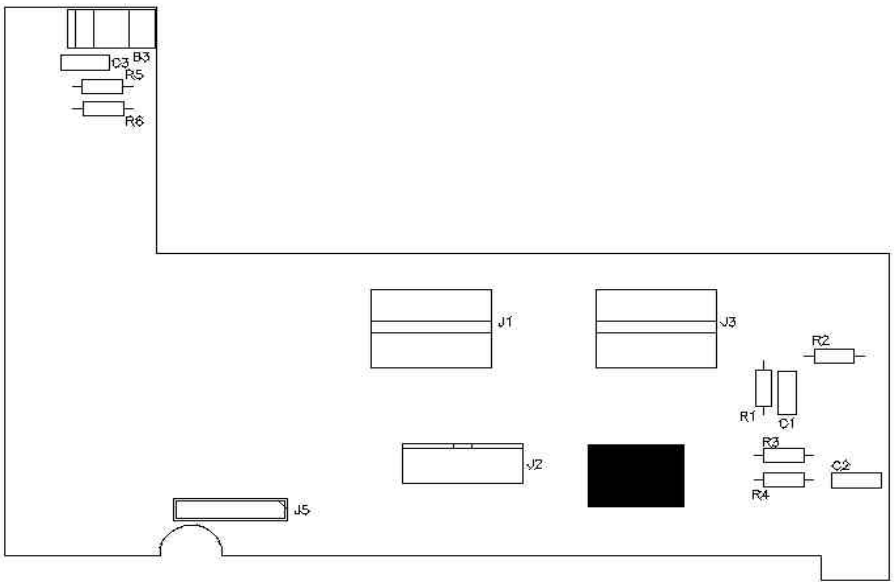

3.6 Communications Board (CIIM00036)

This enables communication with the exterior of the analyzer through a USB channel or a RS232 channel. It also includes an auxiliary RS232 channel for monitoring the functions of the analyzer during its execution.

Connector	Function	Pins
J1	CPU board connection (CIIM00026)	1 - V DC 2 - GND 3 - Tx0 4 - GND 5 - Rx0 6 - GND 7 - GND 8 - Tx1 9 - GND 10 - Rx1

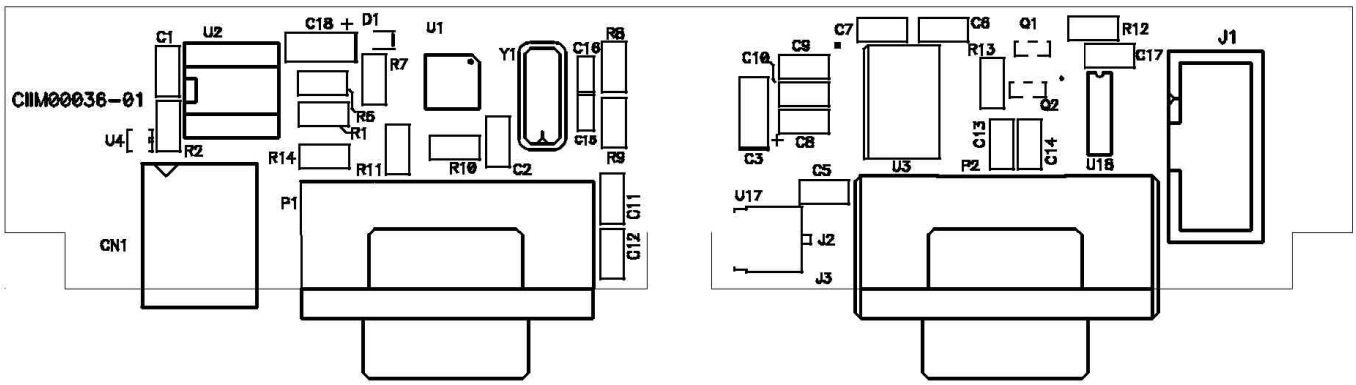

CN1 - USB Connector
P1 - Main RS232 connector
P2 - Auxiliary RS232 connector

3.7 Rotor interconnection board (CIIM00029)

This interconnects the rotor with the CPU board.

Connector	Function	Pins
J1	Rotor motor connection	
J2	Power connection with board CIIM00026	1 - Coil 2 rotor motor 2 - Coil 2 rotor motor 3 - Coil 1 rotor motor 4 - Coil 1 motor filters 5 - Coil 1 rotor motor 6 - Coil 1 motor filters 7 - Peltier 8 - Coil 2 motor filters 9 - Peltier 10 - Coil 2 motor filters 11 - V24 (fans) 12 - GND (fans)
J3	Connection with photometry board CIIM00027	1 - 12 V 2 - GND 3 - DVALID 4 - DCLK 5 - DOUT 6 - DXMIT 7 - RANGE2 8 - RANGE1 9 - RANGE0 10 - TEST 11 - CONV 12 - GND 13 - CLKAD 14 - GND 15 -GND 16 - V DC
J4	Connection motor filters	1 - Coil 1 2 - Coil 1 1 - Coil 2 2 - Coil 2
J5	Peltier connection	1 - Peltier black 2 - Peltier, red
J6	Fan connection	1 - Fan, black 2 - Fan, red
J7	Connection signal with board CIM00026	1 - 12 V 2 - GND 3 - DVALID 4 - DCLK 5 - DOUT 6 - DXMIT 7 - RANGE2 8 - RANGE1 9 - RANGE0 10 - TEST 11 - CONV 12 - GND 13 - CLKAD 14 - GND 15 - GND 16 - V DC 17 - V DC 18 - Rotor cover sensor 19 - GND 20 - Thermistor signal 21 - Home filter drum 22 - GND thermistor 23 - Home rotor 24 - Front LED (red) 25 - Front LED (green) 26 - Ambient sensor

Connector	Function	Pins
J8	Rotor cover sensor connection	1 - Cable 1 2 - Cable 2
J9	Thermistor connection	1 - Cable 1 2 - Cable 2
J10	Front LED connection	1 - Front LED, red 2 - Front LED, black 3 - Front LED, green
J11	Connection Home motor filters	1 - Photo sensor, yellow 2 - Photo sensor, black 3 - Photo sensor, red
J12	Connection Home rotor	1 - Photo sensor, yellow 2 - Photo sensor, black 3 - Photo sensor, red
J13	Connection fans	1 - Fan, black 2 - Fan, red

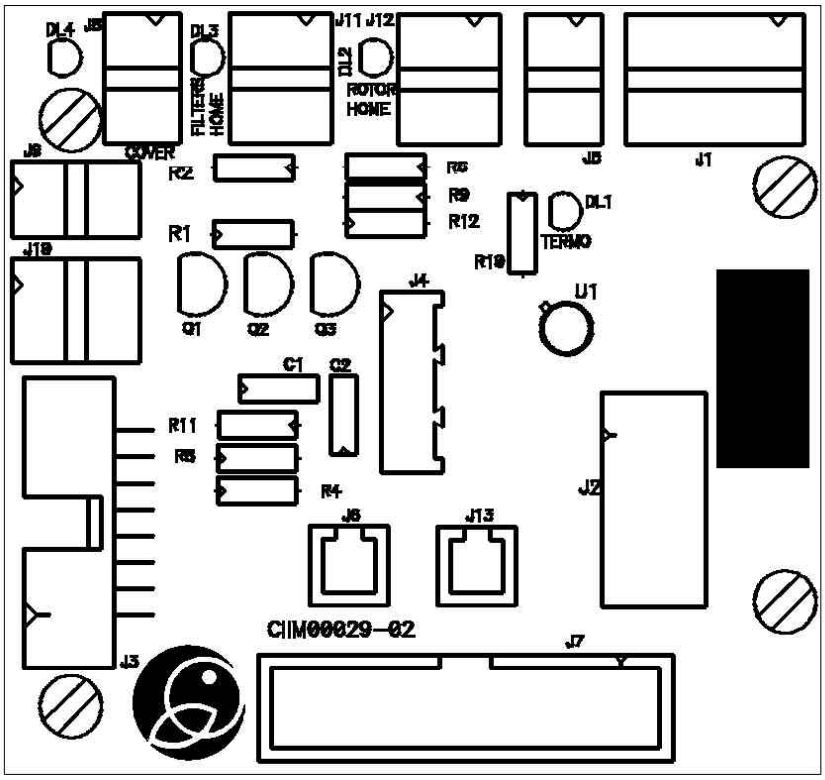

List of LED diodes

DL1 Peltier
DL2 Home rotor motor
DL3 Home filter motor
DL4 Rotor cover

3.9 Pump interconnection board (CIIM00028)

The pump interconnection board interconnects the CPU board with the dispensing pump, the waste pump, the electrovalve, the bottle level sensor and the instrument cover.

Connector	Function	Pins
J1	Waste sensor	1 - Waste sensor
J2	Connection signal with board CIIM00026	1 - Waste sensor 2 - System liquid sensor 3 - LS/waste signal 4 - Needle liquid detection signal 5 - Home dispensation pump 6 - V DC 7 - GND 8 - Instrument cover
J3	System liquid sensor	1 - System liquid sensor
J4	LS/waste sensor signal	1 - System liquid signal
J5	Needle liquid detection signal	1 - Needle liquid detection signal
J6	Dispensation pump home	1 - Photo sensor, yellow 2 - Photo sensor, black 3 - Photo sensor, black
J7	Electrovalve	1 - White cable 2 - White cable
J8	Power connection with board CIIM00026	1 - 24 V electrovalve 2 - GND 3 - Waste pump 4 - Waste pump 5 - Dispensation pump coil 1 6 - Dispensation pump coil 1 7 - Dispensation pump coil 2 8 - Dispensation pump coil 2
J9	Waste pump	1 - Waste pump, red 2 - Waste pump, black
J10	Waste pump	1 - Coil 1 2 - Coil 1 4 - Coil 2 5 - Coil 2
J11	Instrument cover	1 - Photo sensor, yellow 2 - Photo sensor, black 3 - Photo sensor, red

List of LED diodes

DL1 Electrovalve
DL2 Waste pump
DL3 Home pump
DL4 Instrument cover

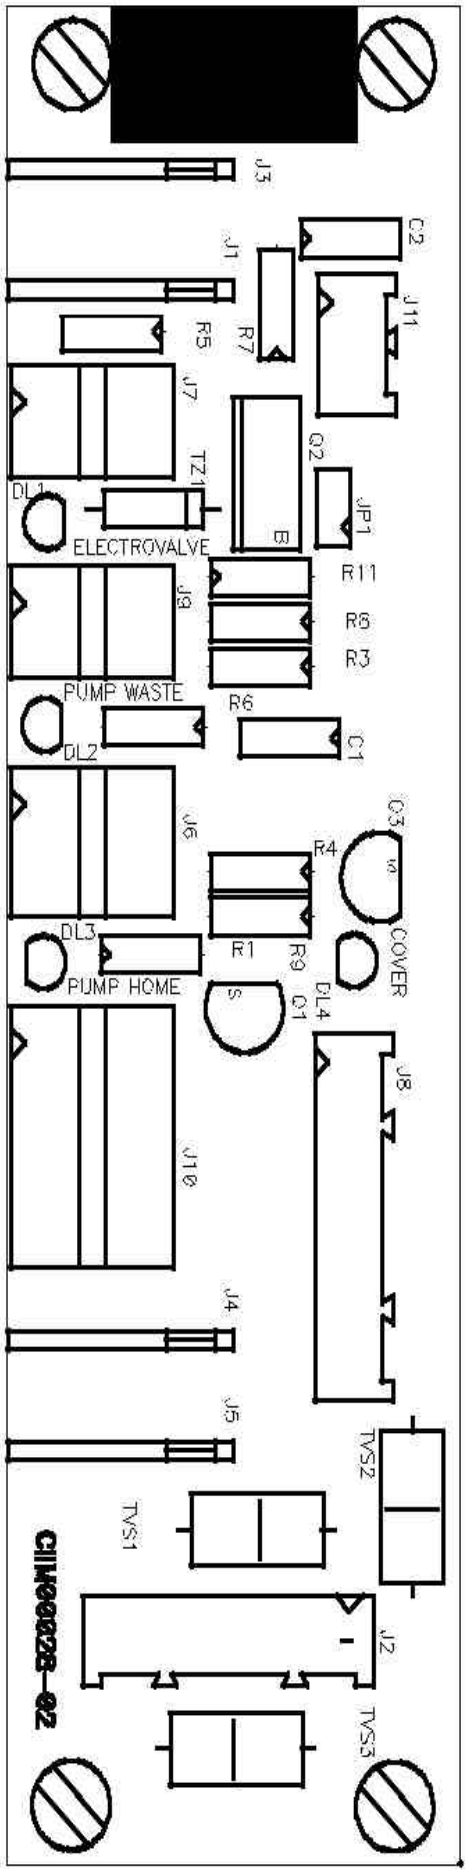
J3
C2
J1
J11
R5
R7
J7
Q2
TZ1
DL1
JP1
ELECTROVALVE
B
R11
J9
R6
R3
PUMP WASTE
R6
DL2
C1
J6
Q3
R4
DL3
R1
R9
COVER
PUMP HOME
S
Q1
DL4
J8
J10
J4
J5
TVS2
TVS1
J2
TVS3

3.10 Interconnection between boards

The following diagrams show the connections between the boards and the different elements that make up the analyzer.

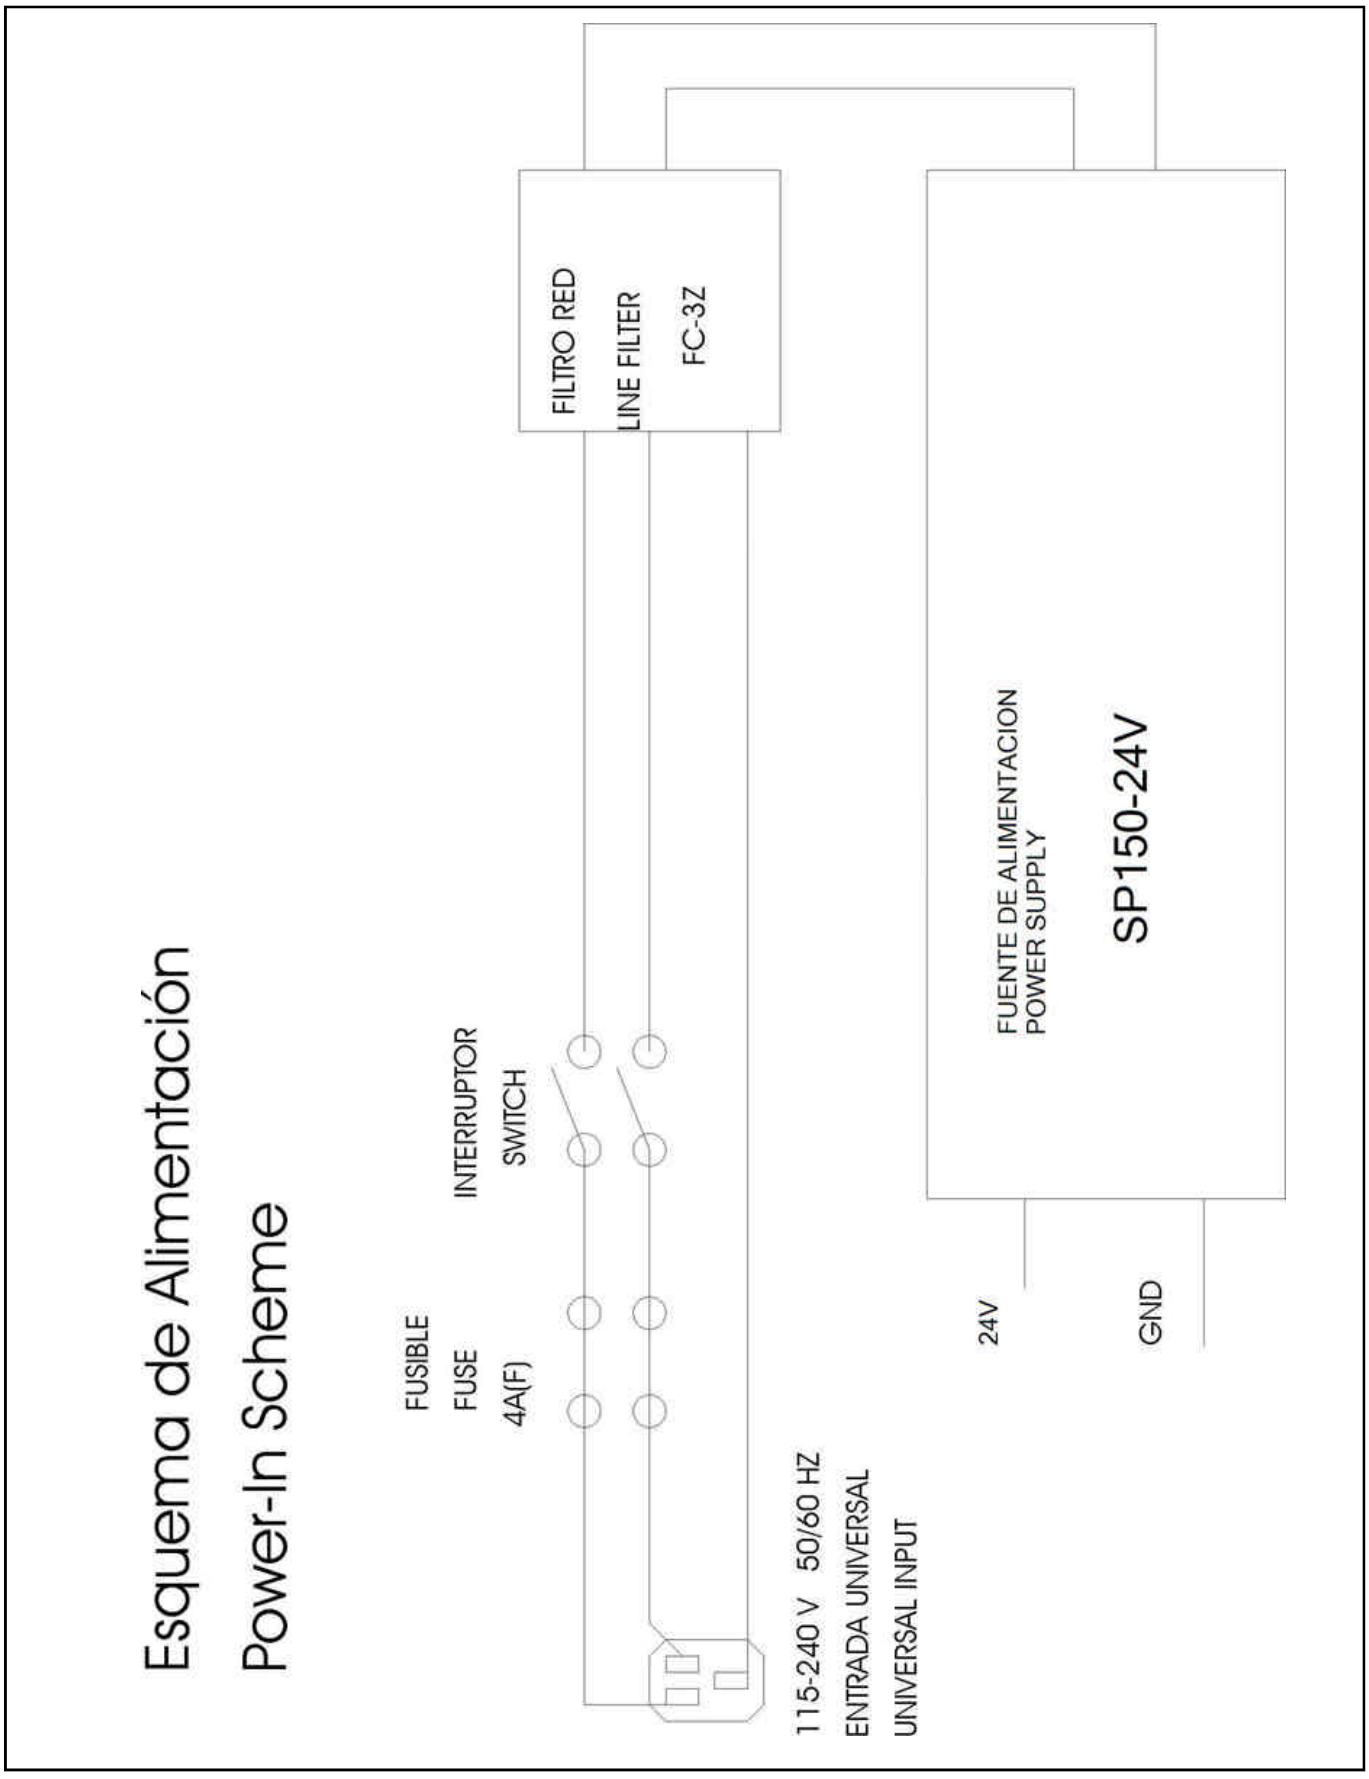

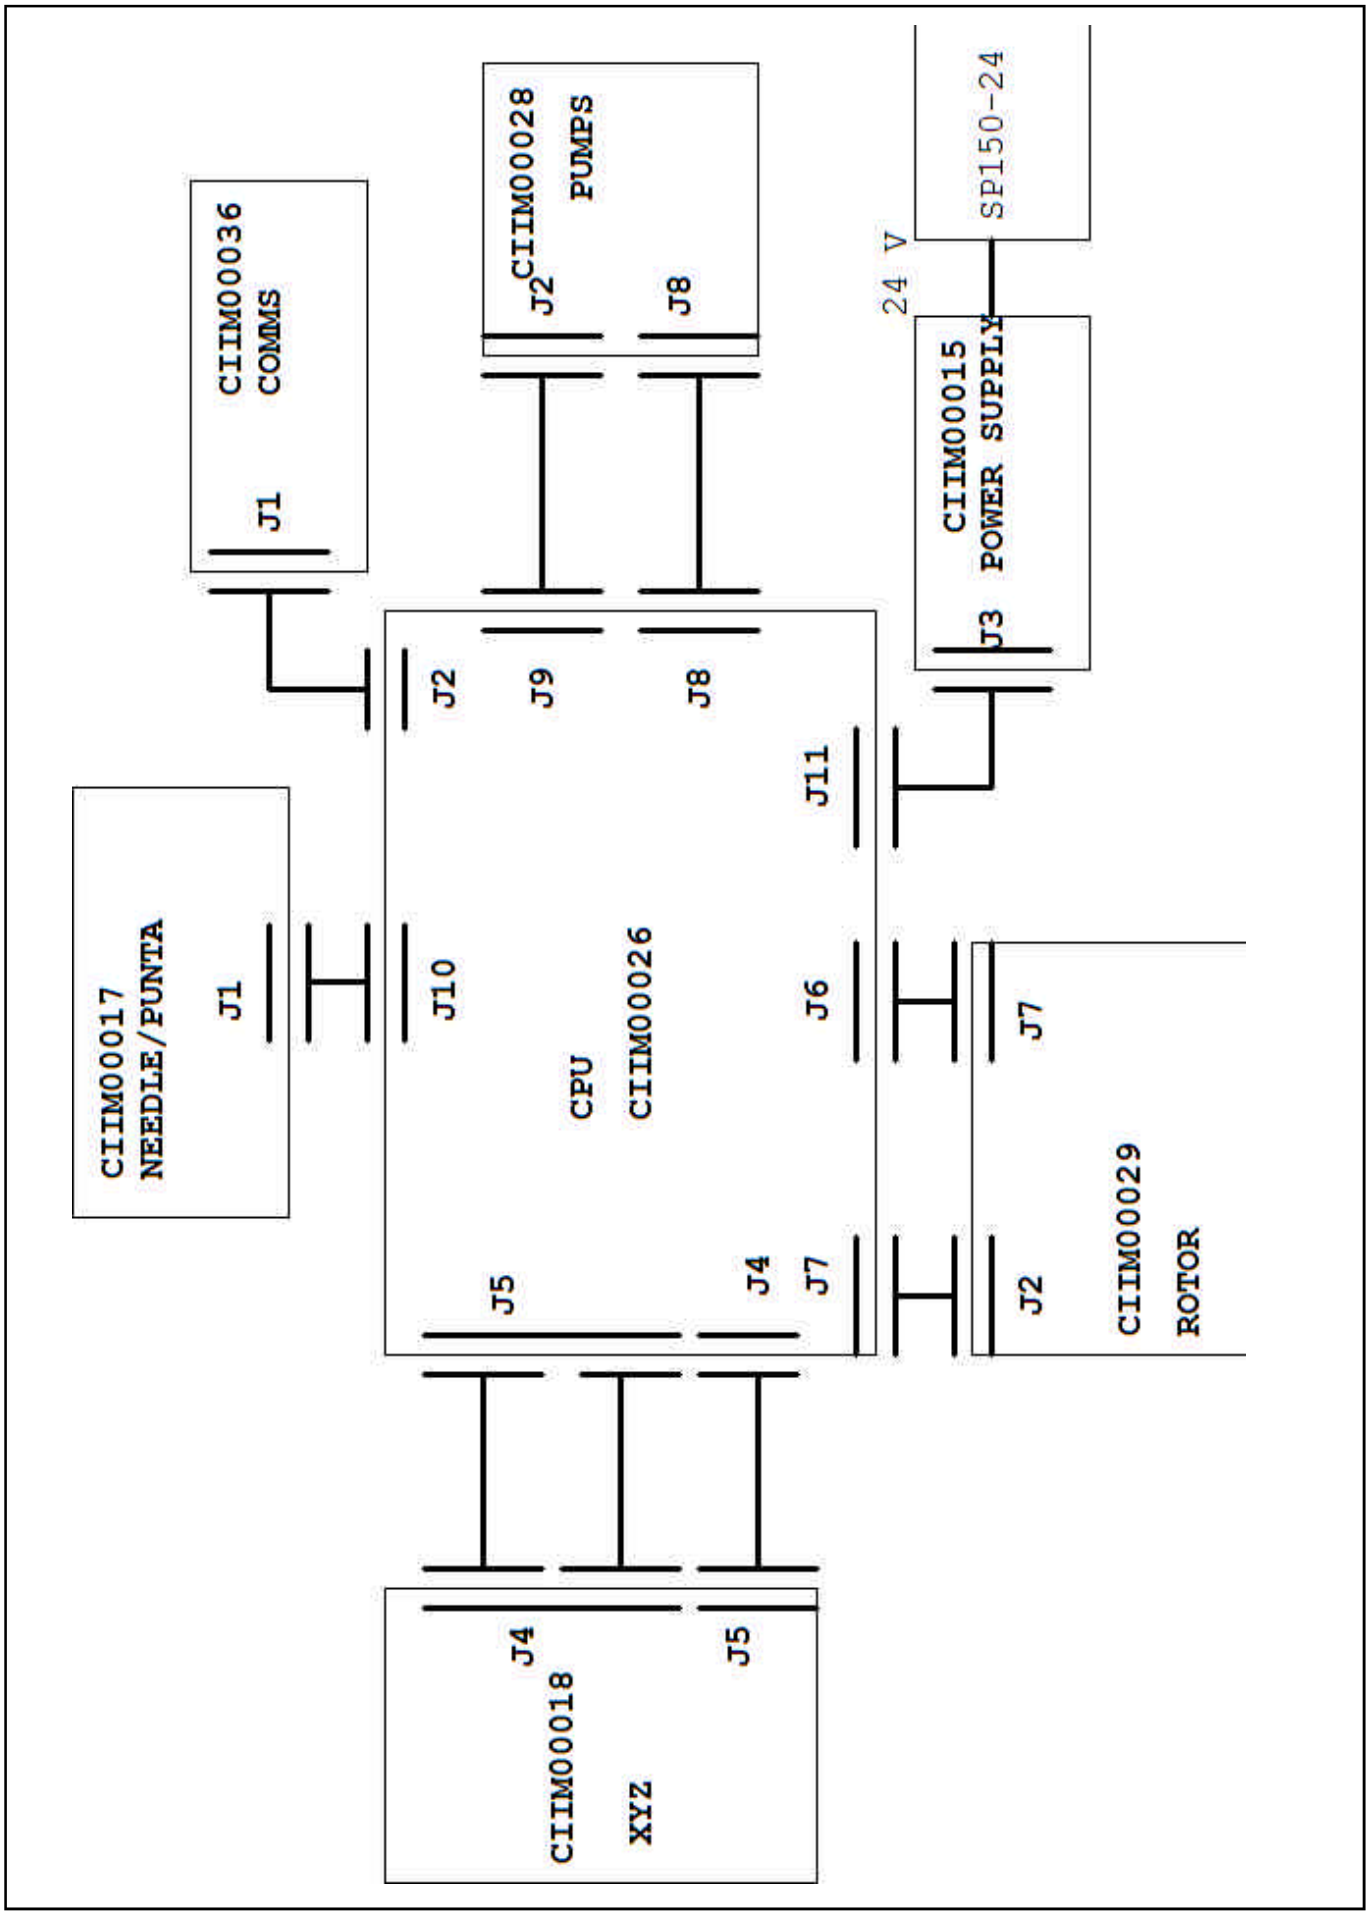
CIIM00036
COMMS
J1
CIIM00028
PUMPS
J2
J8
24 V
SP150-24
CIIM00015
POWER SUPPLY
J3
CIIM00017
NEEDLE/PUNTA
J1
J2
J9
J8
J11
J10
CPU
CIIM00026
J6
J7
J5
J4
J7
J2
CIIM00029
ROTOR
J4
J5
CIIM00018
XYZ

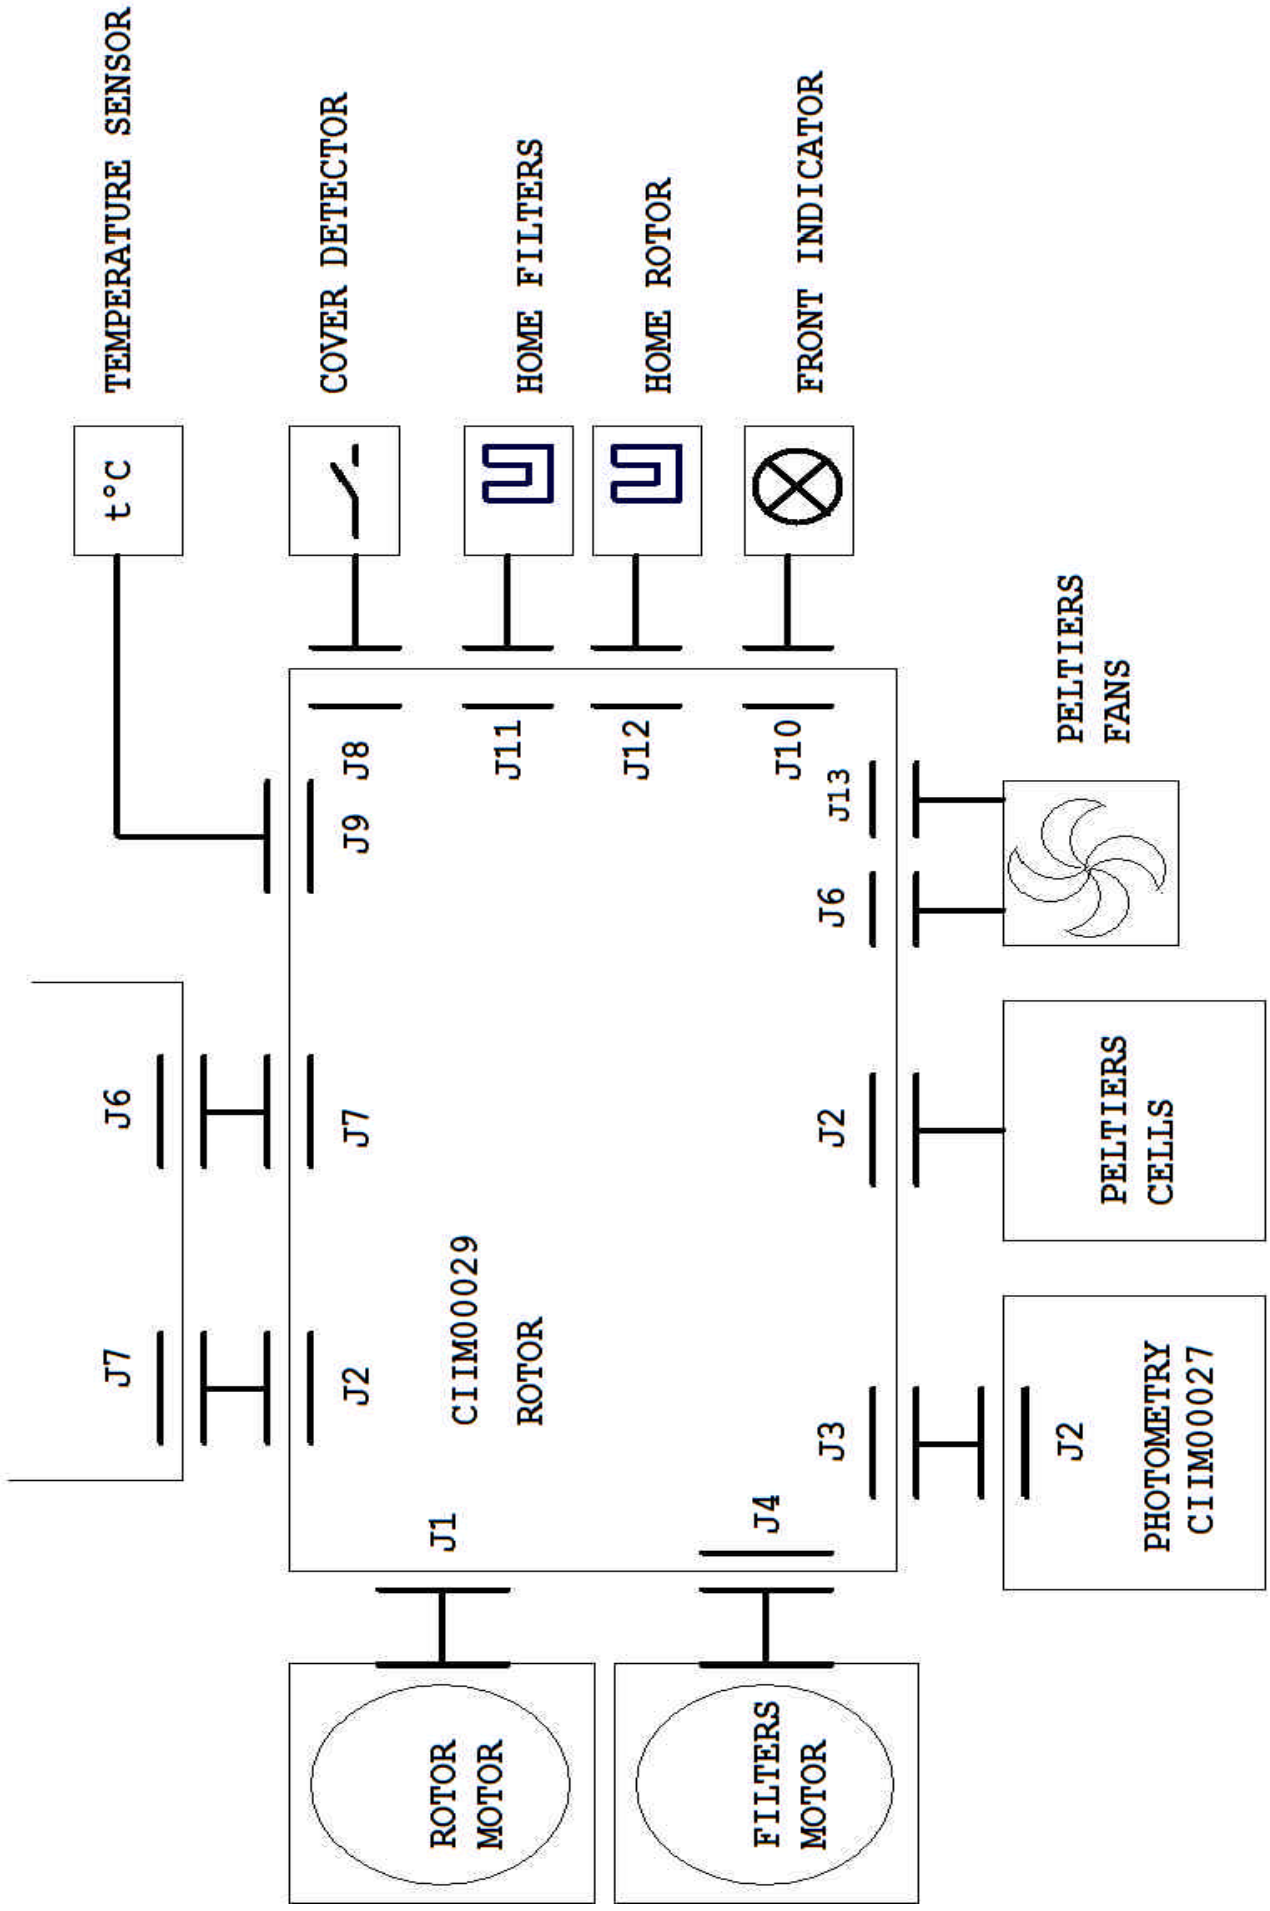
TEMPERATURE SENSOR
COVER DETECTOR
HOME FILTERS
HOME ROTOR
FRONT INDICATOR
t°C
J8
J9
J11
J12
J10
J13
J6
PELTIERS
FANS
J6
J7
J7
J2
CIIM00029
ROTOR
J2
PELTIERS
CELLS
J1
J4
J3
J2
PHOTOMETRY
CIIM00027
ROTOR
MOTOR
FILTERS
MOTOR

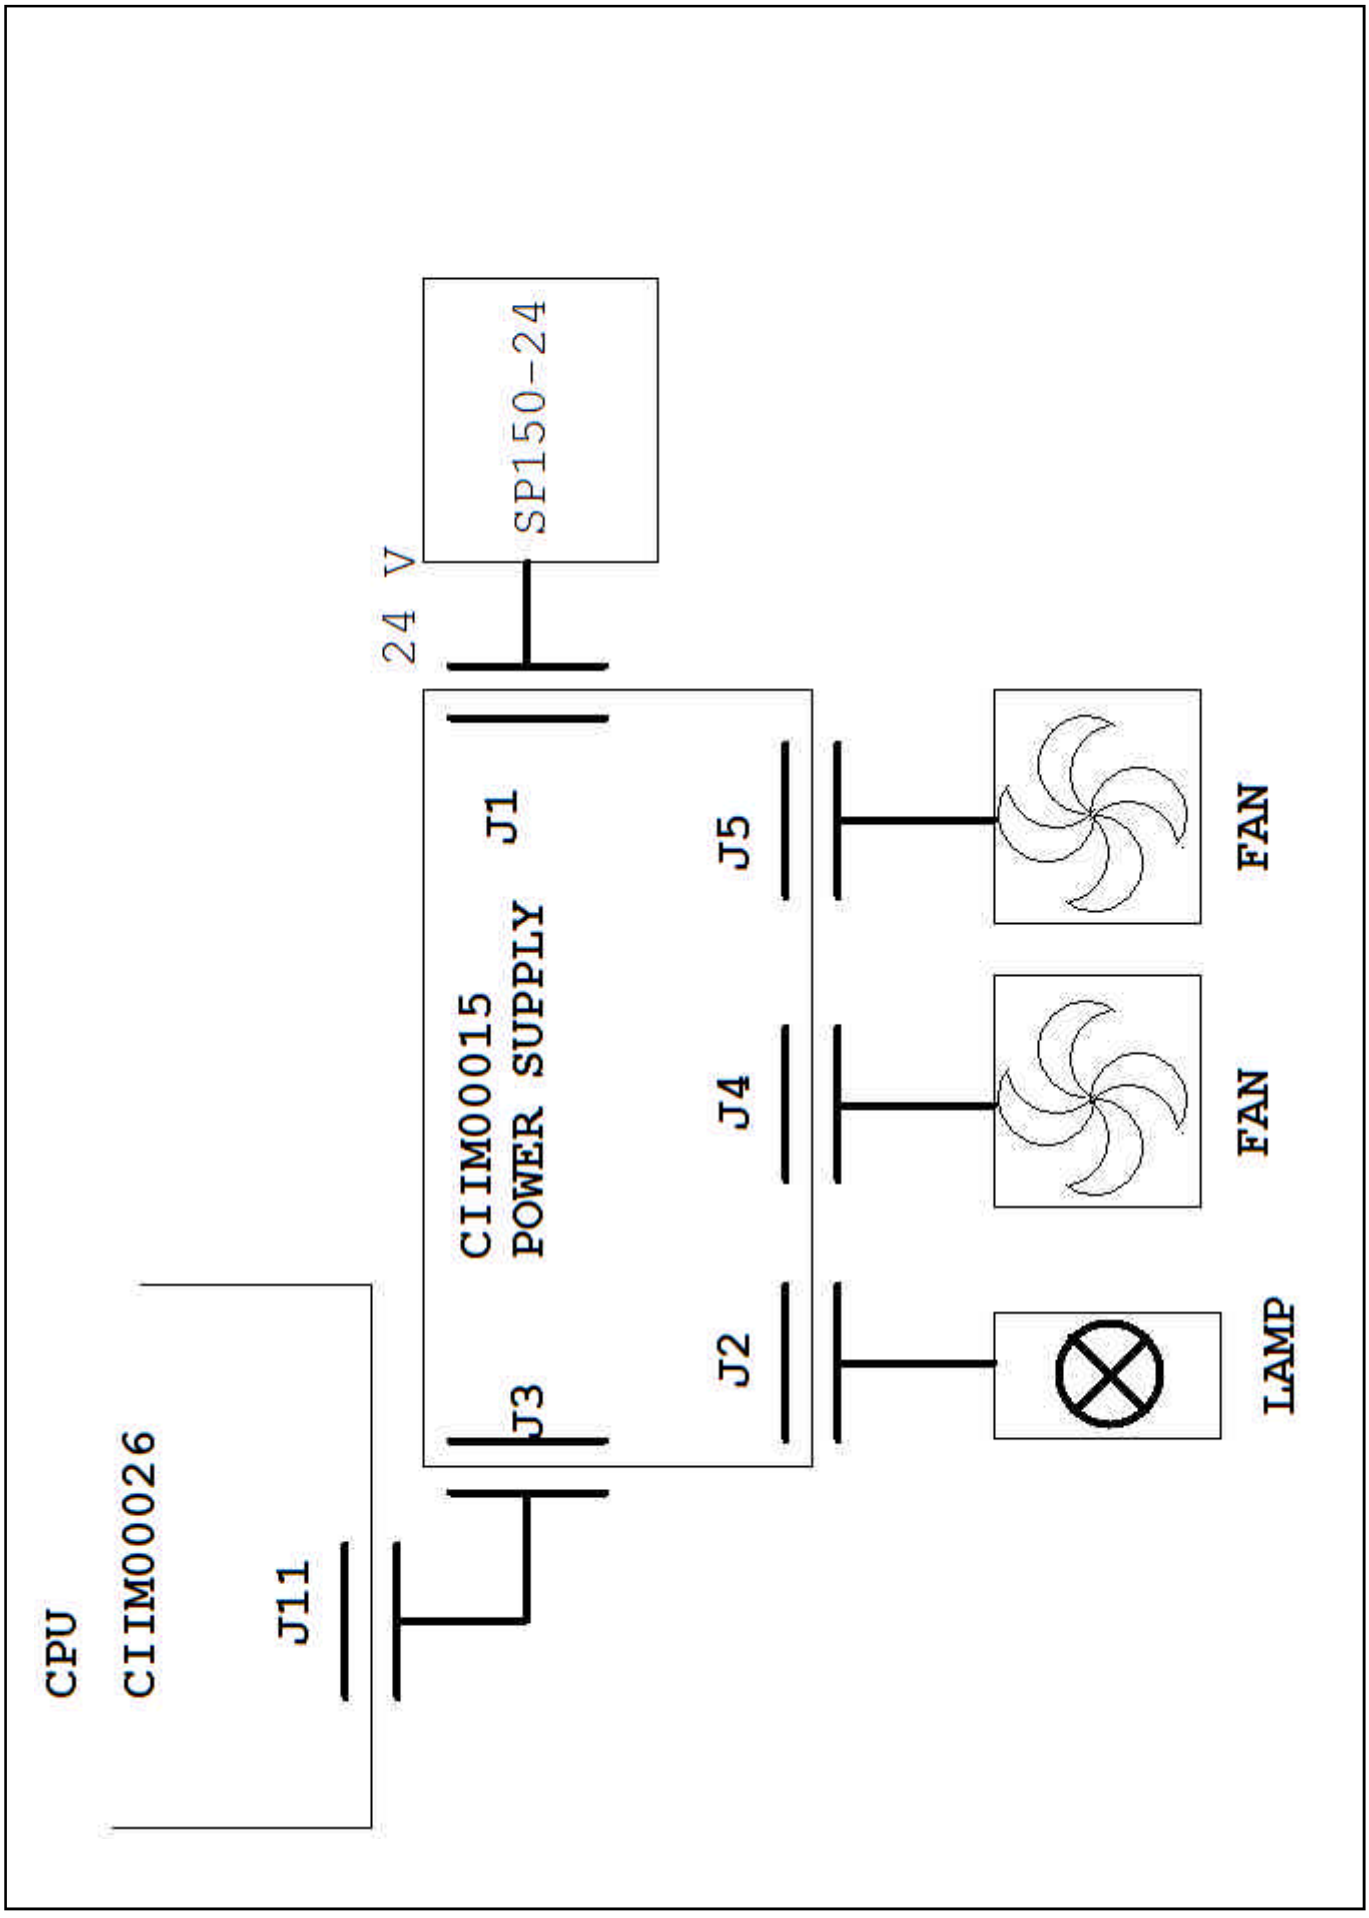
CPU
CIIM00026
J11
J3
CIIM00015
POWER SUPPLY
J1
24 V
SP150-24
J2
J4
J5
LAMP
FAN
FAN

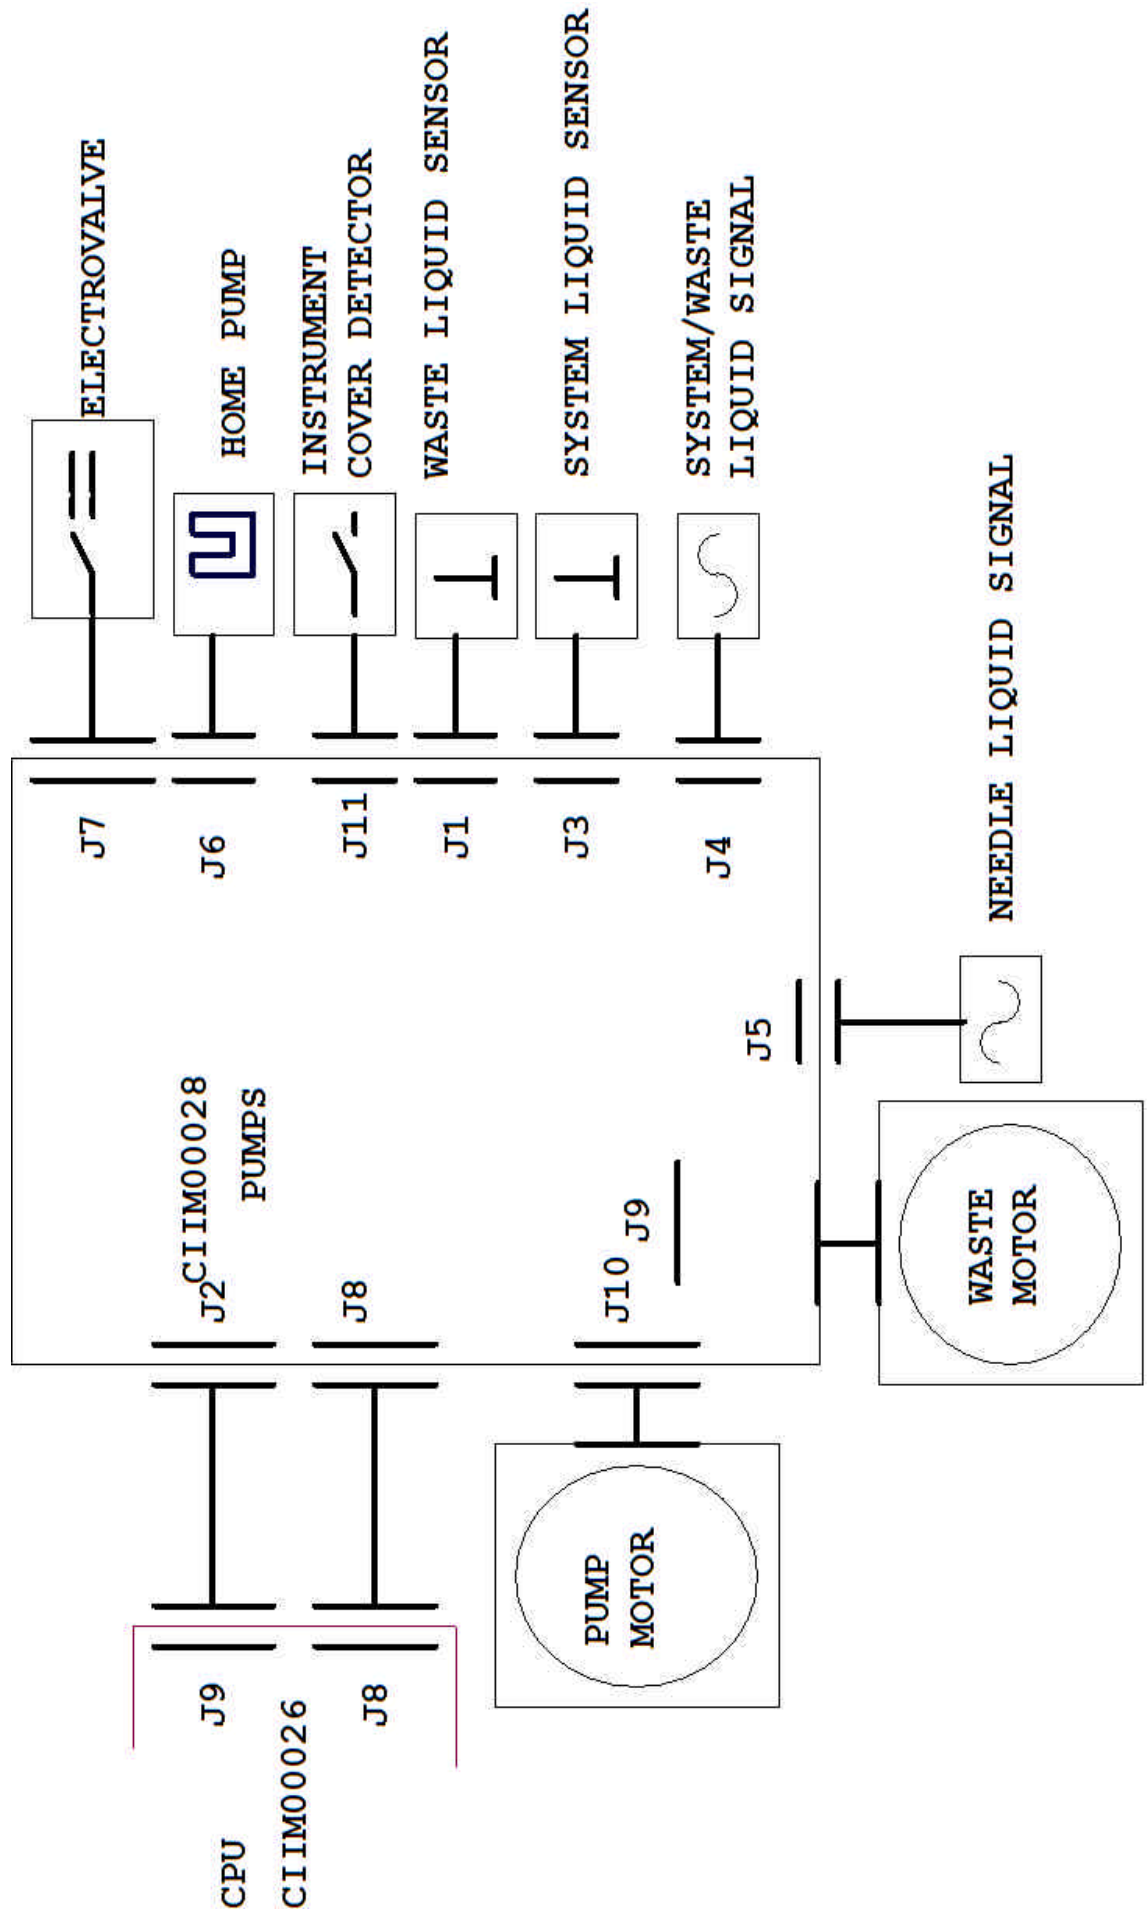
ELECTROVALVE
HOME PUMP
INSTRUMENT
COVER DETECTOR
WASTE LIQUID SENSOR
SYSTEM LIQUID SENSOR
SYSTEM/WASTE
LIQUID SIGNAL
NEEDLE LIQUID SIGNAL
J7
J6
J11
J1
J3
J4
J5
J2
CIIM00028
PUMPS
J8
J10
J9
WASTE
MOTOR
PUMP
MOTOR
J9
J8
CPU
CIIM00026

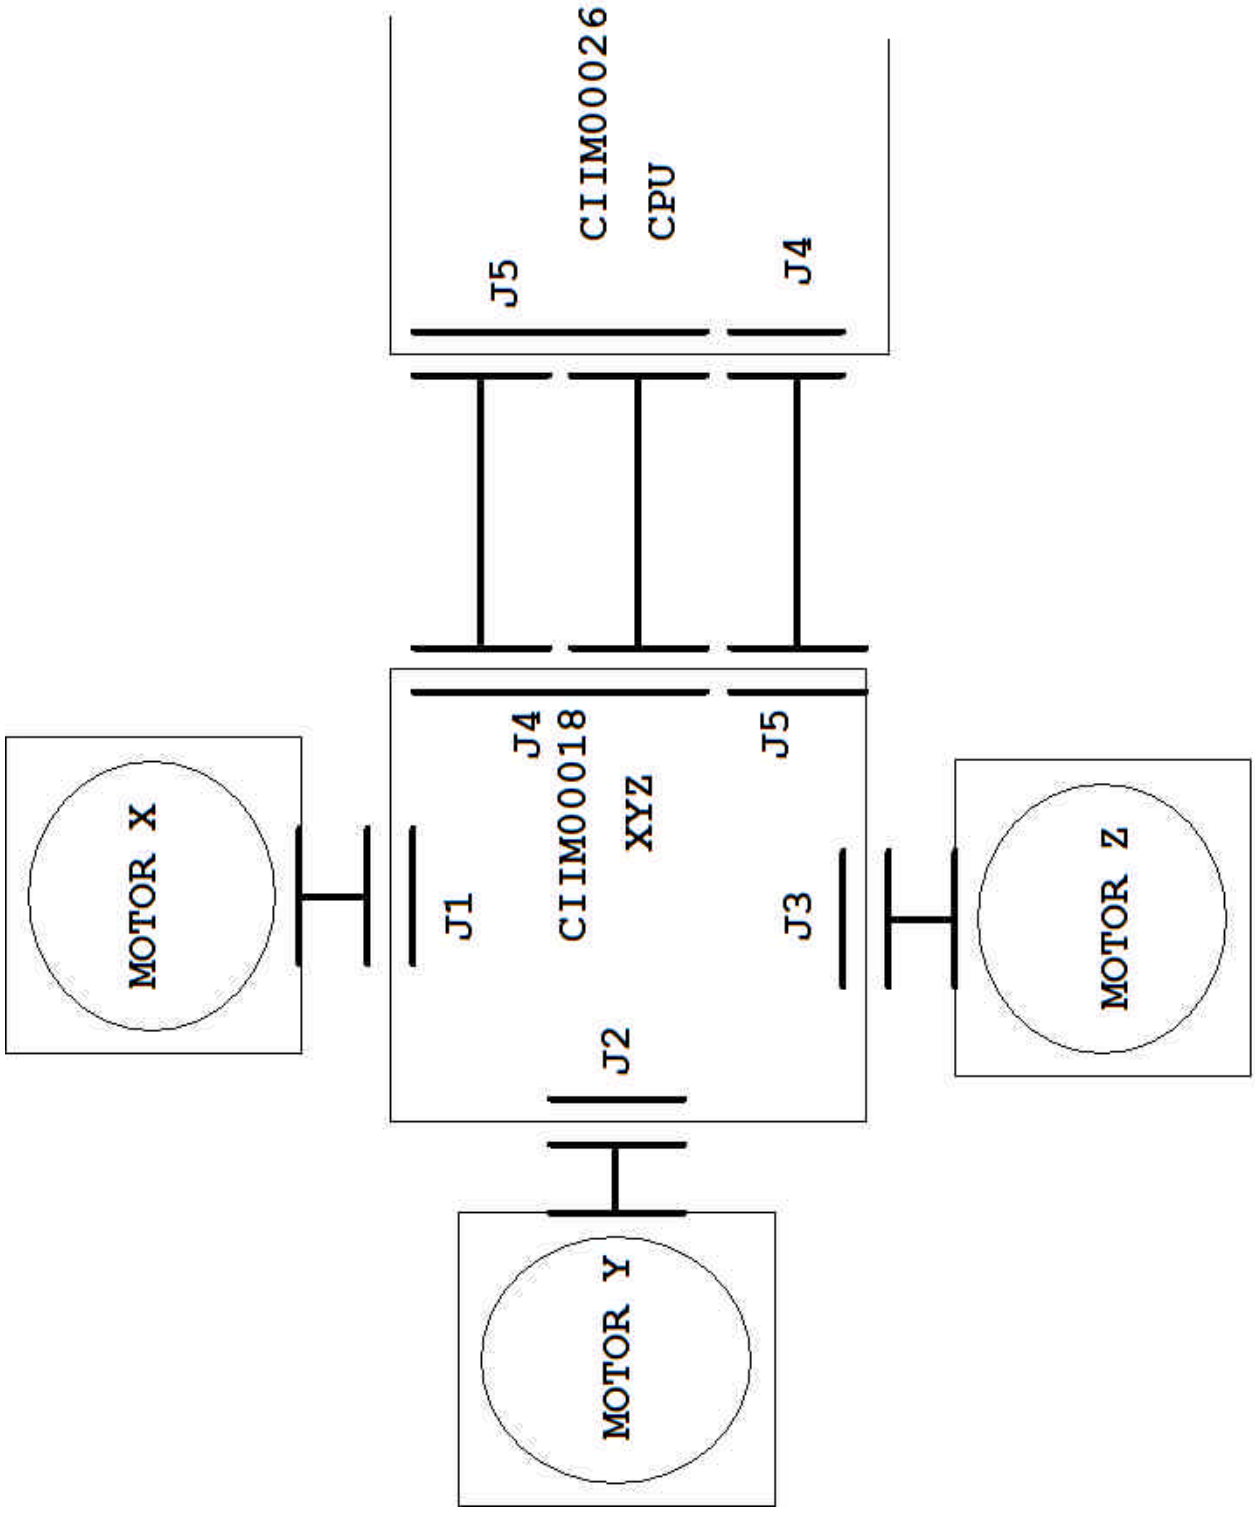
CIIM00026
CPU
J5
J4
CIIM00018
XYZ
J4
J5
J1
J3
J2
MOTOR X
MOTOR Z
MOTOR Y

4. SERVICE PROGRAM

The service program is used for the adjustment, checking and maintenance of the different components of the analyzer. It is not supplied with the instrument, it is supplied to authorised technical services only. The personal of the Technical Service must install it on the user's computer in order to carry out the service requirements. Once the tasks have finalised, the program must be uninstalled. To install the program, follow the instructions on the installation CD ROM called *Service*. The original password for using this program is ***A15***. The password can be changed from the service program itself. If the service personnel forget the password, the original password can be reinstalled by deleting the hidden file *code.A15* from the application directory and relaunching the program. Once the password has been introduced, the analyzer serial number is given and the name of the operator is requested (by default *Operator1*). Press the *Accept* button and the main program appears. The different functions of the service program are classified in the following categories:

- **Adjustments**: These make it possible to make different parameter adjustments required for the correct functioning of the analyzer.
- **Tests**: Tests for checking the functionality of the analyzer.
- **Utilities**: Different technical utilities, such as, for example, washing or priming the dispensing system or changing an optical filter.
- **Registers**:This enables the management of past adjustments, tests, incidences, repairs and maintenance of the instrument.
- **Monitor**:These enable the low level communication with the analyzer to load new versions of the program in the *flash* memory of the analyzer (*firmware*) or to consult the internal parameters of the instrument.

An emergency stop button (*STOP on a red background*) will be accessible at all times, and when pressed, it switches off the analyzer and closes the application quickly.

4.1 Initialising the analyser

To initialise the analyser in service mode, first launch the A15 Service application. The program first of all requests a user or technician ID to be used in the program. Depending on the type of user identified, access to the different parts of the program will be allowed or denied. The following screen appears:

For full access, enter the following codes:
Name (login): ***SAT***
Password: ***A15***

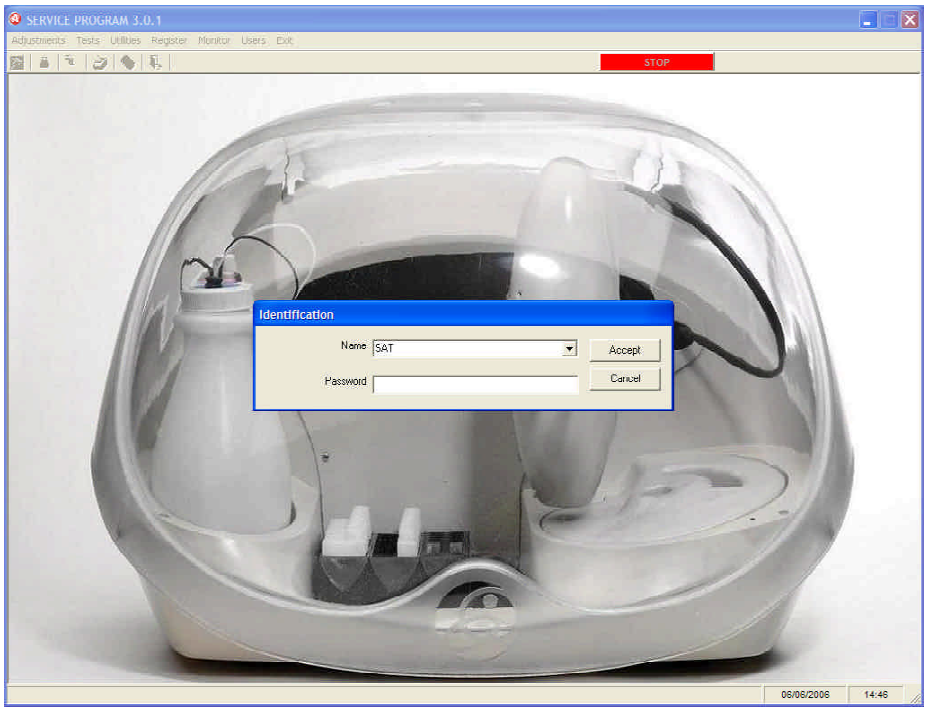

Once the user has been identified correctly, the service program starts to initialise the analyser.

This screen appears when the analyser has finished the previous operations done to enter the SERVICE mode. If the complete hardware of the analyzer is in correct conditions, the result “Hardware initiated correctly» displays. If any hardware element presents an operational problem, it will appear “Hardware not initiated completely” in the screen, and the element that is not working correctly will be shown.
In order to close the screen and continue working, you should press the *Accept* button.
In order to get a printed copy of this initialization report, you should press the *Print* button.
NOTE: If an error has been reported and the technician continues working with the service program, he must consider that there is a hardware element that is not working properly.

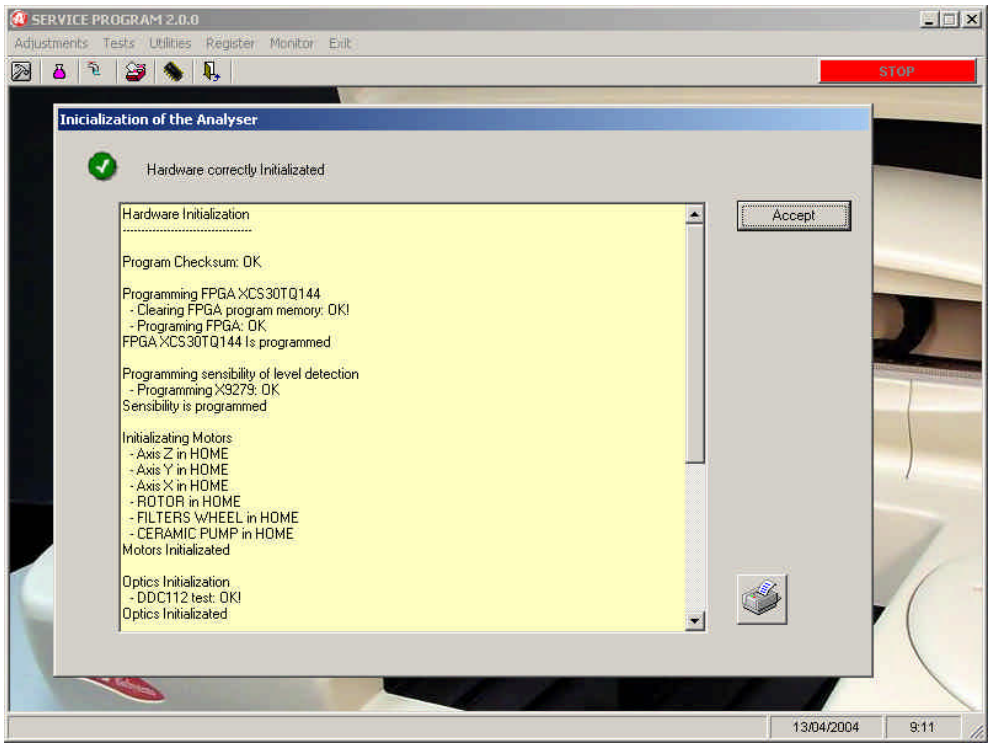

A25 SERVICE PROGRAM 1.5
Adjustments Tests Utilities Register Monitor Exit
STOP
EMERGENCY STOP! Program Service and the analyzer will be shutting down
02/10/2003
12:21

4.2. ADJUSTMENTS

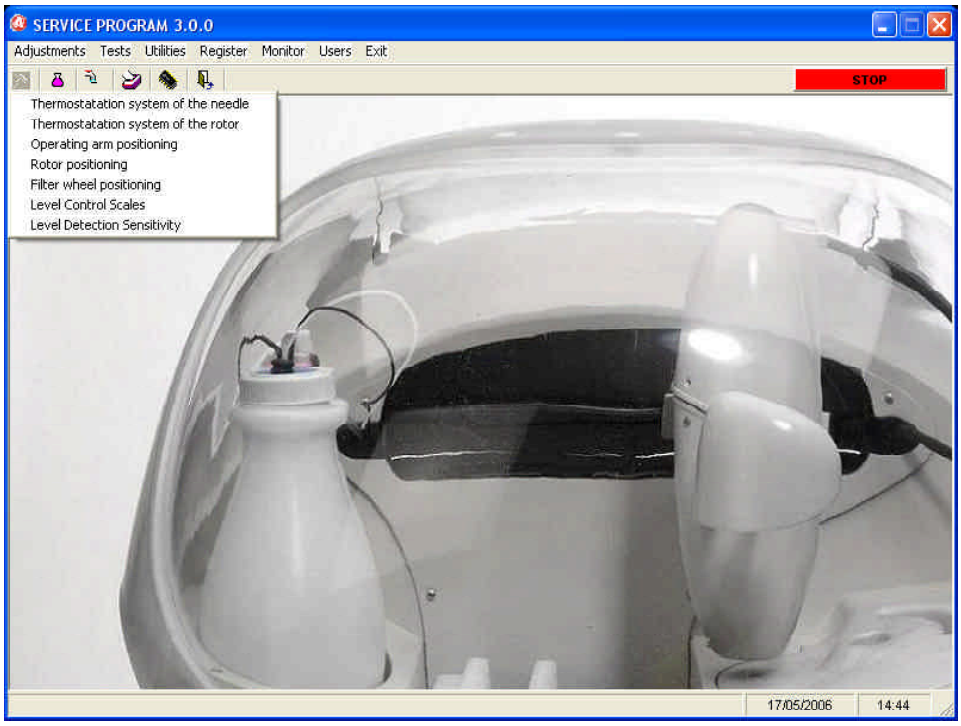

These make it possible to make different parameter adjustments required for the correct functioning of the analyzer. All the values to be adjusted have certain limited ranges, indicated by the service program. These values are also given in an appendix at the back of this manual. If, after varying any of the parameters within its permitted range, the analyzer is not tuned up, it indicates that the corresponding system is broken and in need of repair.

4.2.1. Adjustment of the needle thermostatation system

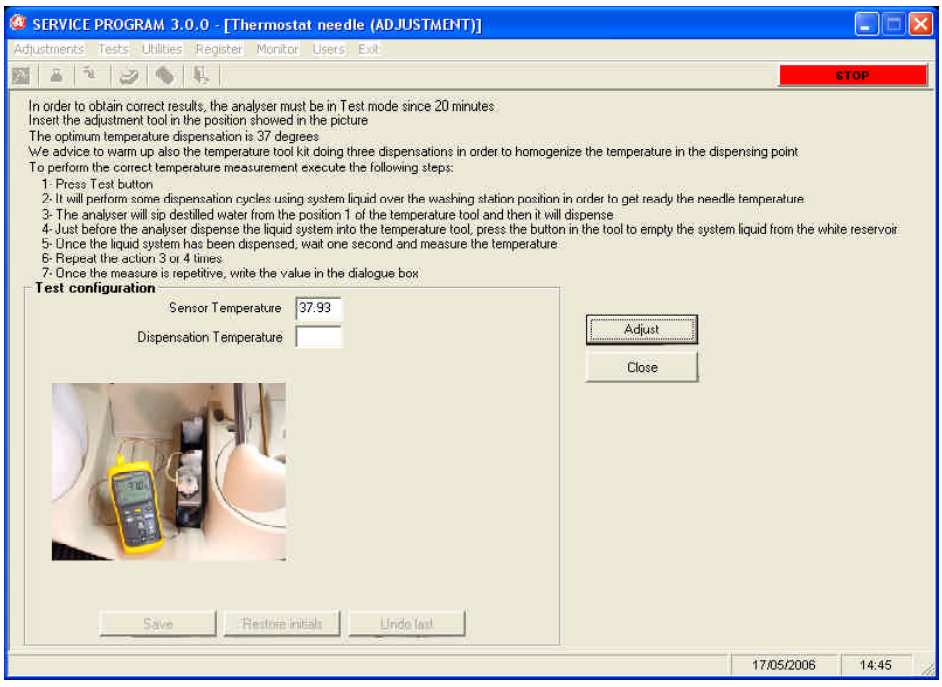
SERVICE PROGRAM 3.0.0 - [Thermostat needle (ADJUSTMENT)]
Adjustments Tests Utilities Register Monitor Users Exit
STOP
In order to obtain correct results, the analyser must be in Test mode since 20 minutes
Insert the adjustment tool in the position showed in the picture
The optimum temperature dispensation is 37 degrees
We advice to warm up also the temperature tool kit doing three dispensations in order to homogenize the temperature in the dispensing point
To perform the correct temperature measurement execute the following steps:
1- Press Test button
2- It will perform some dispensation cycles using system liquid over the washing station position in order to get ready the needle temperature
3- The analyser will sip destilled water from the position 1 of the temperature tool and then it will dispense
4- Just before the analyser dispense the liquid system into the temperature tool, press the button in the tool to empty the system liquid from the white reservoir
5- Once the liquid system has been dispensed, wait one second and measure the temperature
6- Repeat the action 3 or 4 times
7- Once the measure is repetitive, write the value in the dialogue box
Test configuration
Sensor Temperature
37.93
Dispensation Temperature
Adjust
Close
Save
Restore initials
Undo last
17/05/2006
14:45

This screen adjusts the needle thermostatation in such a way that the dispensing temperature of the reactions is as close as possible to 37ºC. To make this adjustment, the analyzer must be initialised. The liquid to be dispensed is taken from the system liquid container or from the bottle of reagent selected by the technician. The technician must measure the temperature of the dispensed liquid with a thermometer calibrated at 37ºC. The program shows the control set point temperature, which is the parameter that must be adjusted for the dispensing temperature to be correct. This parameter must be different from 37ºC. When the technician so indicates, the analyzer dispenses thermostated distilled water on a certain position in the racks tray shown on the screen. The technician must measure the temperature of the water with the calibrated thermometer and introduce the temperature on the screen. The analyzer automatically modifies the set point temperature in accord with the temperature measured with the thermometer for the dispensing temperature to be 37ºC. The technician can modify this set point temperature proposed by the program. On pressing *Adjust*, the analyzer thermostates the needle with the new set point and, when the technician so requests, performs new dispensing operations. Each time the set point temperature is modified, wait 1 minute before performing new dispensing operations for the needle temperature to become stabilised. The technician must repeat this process until the dispensing temperature is as near as possible to 37ºC. Pressing the *Store* button, the analyzer stores the current value of the adjusted set point temperature. Pressing the *Cancel* button keeps the last stored value and the current value is not stored. Pressing the *Restore* button restores the initial screen input value.

4.2.2. Adjustment of the rotor thermostation system

This screen makes it possible to adjust the thermostation system of the rotor in such a way that the reactions temperature is 37ºC. To make this adjustment, place a well rotor in position and ensure that the analyzer has been initialised. The rotor can be automatically filled with distilled water by pressing the corresponding button. Once filled, the technician must wait a few minutes for the rotor to be thermostated. The temperature in the rotor wells must be measured with a temperature calibrated at 37ºC through the dispensing hole of the rotor cover. A button makes it possible to turn the rotor in increases of 15 wells to change the well on which the measurement is being taken. The program shows the control set point temperature, which is the parameter that must be adjusted for the temperature of the rotor to be correct. This parameter must be other than 37ºC. The technician must measure the temperature of the water with the calibrated thermometer in the wells and enter the temperature on the screen. The analyzer automatically modifies the set point temperature in accord with the temperature measured with the thermometer for the rotor reactions temperature to be 37ºC. The technician can modify this set point temperature proposed by the program. On pressing *Adjust*, the analyzer thermostates the rotor with the new set point. Each time the set point temperature is modified, wait 5 minutes before performing new dispensing operations for the rotor temperature to become stabilised. The technician must repeat this process until the rotor temperature is as near as possible to 37ºC. Pressing the *Store* button, the analyzer stores the current value of the adjusted set point

SERVICE PROGRAM 3.0.0 - [Rotor Thermostatation (ADJUSTMENT)]
Adjustments
Tests
Utilities
Register
Monitor
Users
Exit
STOP
REMEMBER: You must have performed the Warming Up for the measurements to be significant.
After filling the rotor, wait 5 to 10 minutes for the liquid to reach its final temperature.
You must wait every time the sensor temperature is modified.
To check the homogeneity of the temperature inside the rotor, measurements have to be made in the different positions.
The final result is calculated from the average of all the wells temperatures measured. The optimum temperature of the liquids is 37 degrees
Due to the structure of the reactions rotor, the measurement in position 1 is lower. The Analyzer corrects it automaticly.
Rotor filling
Insert a manually filled rotor
Automatic rotor filling by the analyzer
Apply
Test configuration
Sensor temperature
38.43
Average measured temperature
Rotor measurement position
1
Do Measurement
Adjust
Close
Save
Restore initials
Undo last
Before measuring, wait from 5 to 10 minutes for the liquid in the rotor to reach an estable temperature
17/05/2006
14:46

temperature. Pressing the *Cancel* button keeps the last stored value and the current value is not stored. Pressing the *Restore* button restores the initial screen input value.

4.2.3. Adjustment of the positioning of the operating arm

This screen makes it possible to adjust the horizontal positioning (X, Y) of the arm. The arm housing must be removed to see the position of the needle. Before making the adjustments, visually check the verticality of the needle. If necessary, carefully straighten it up ensuring you do not damage it. On the screen, select the point at which you wish to adjust the horizontal positioning. On pressing the *Adjust* button the arm initialises and positions itself over said point. The technician has buttons to move the arm step by step over the horizontal plain (X, Y) and vertically (Z). The arm can also be moved introducing a certain number of absolute movement steps. These absolute movements of the arm must be made with the needle at its highest position so as not to damage it (coordinate 0). The technician must lower the needle to the adjustment point and adjust its horizontal position. When the position is satisfactory, save the current coordinates (X, Y) by pressing the *Store* button. Pressing the *Cancel* button keeps the last adjustment values stored. Pressing the *Restore* button restores the initial screen input values. At all times, the screen shows the current coordinates of the arm for the selected point, the last coordinates stored and the initial screen input coordinates, as additional information for the technician. The technician may repeat the procedure to adjust the positioning of the arm at the different possible adjustment points. These points are as follows:

(1) Origin. Vertex of the self-centering plate of the needle.
(2) Rack tray Adjust point located in the right part at rear of the tray
(3) Washing station. Centre of front part of washing station.
(4) Reactions rotor. Dispensing point on the rotor reactions cover.
(5) Zmax (on tray reference) The same point of rack tray

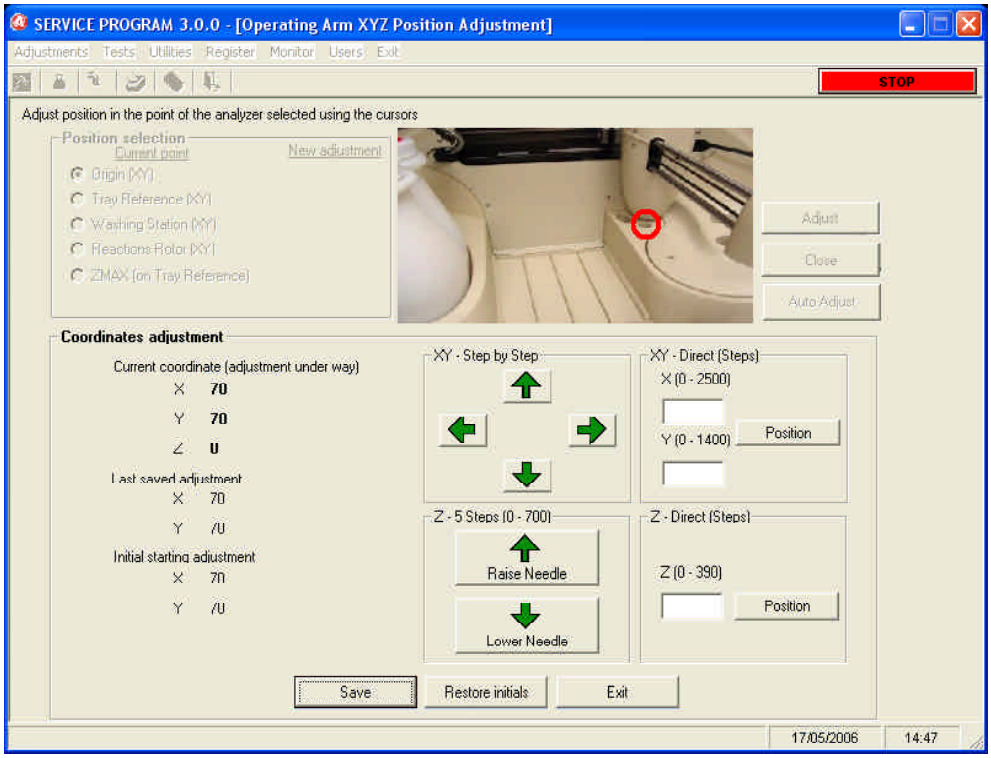

If you select the point of origin, automatic adjustment is possible in this position by pressing an AutoAdjustment button (the process can take around 3 minutes).

4.2.3.1 Adjusting the maximum sweep of the Z axis.

This adjustment prevents the needle from colliding with the rack tray and minimises the zero volume of reagents and samples.

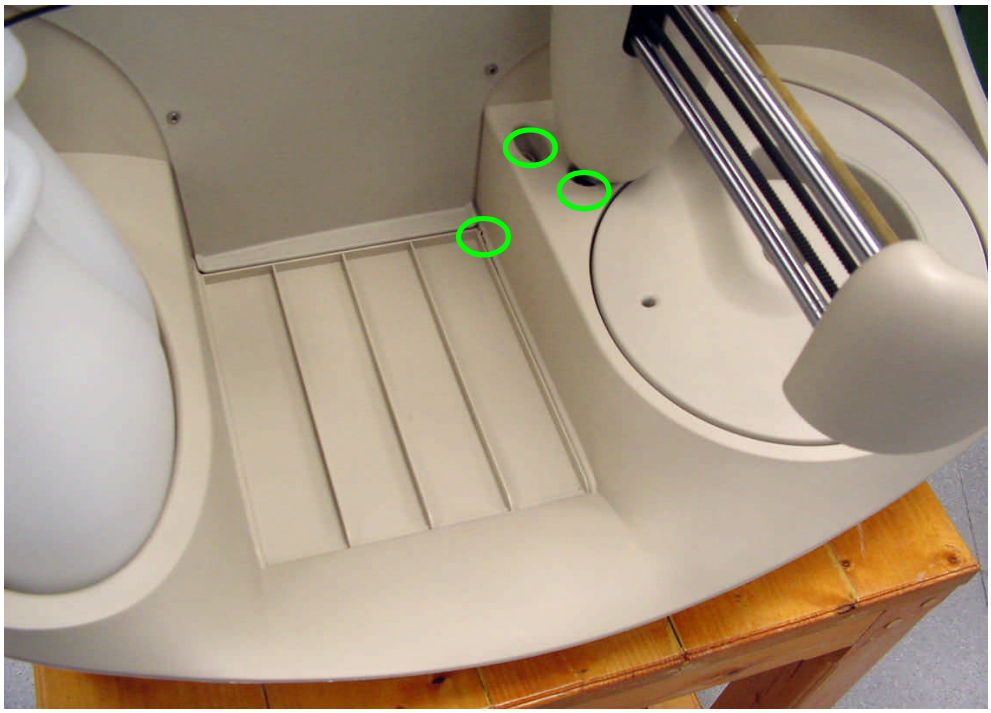

The adjustment is separated into two parts: (1) the adjustment of the maximum sweep; (2) fine tuning (offsets) by rack type.

- Part 1 adjusts the needle to thetray adjust point (same position as the adjustment of the rack tray reference). This adjustment consists of moving the nee dle until it comes into contact with the adjust point on the rack tray. This operation can be completed by moving the needle to an absolute Z coordinate, Z-direct box, and then using the *needle up* and *needle down* keys until contact is made with adjust point. The programme then calculates the real reference by adding a constant value so that the needle is lowered to the rack position. Bear in mind that the encoder detection of the needle is not enabled. Consequently, if there is a collision by entering a high value in the Z-direct box, it may collide with the adjust point. In this case, use the *Home* button to

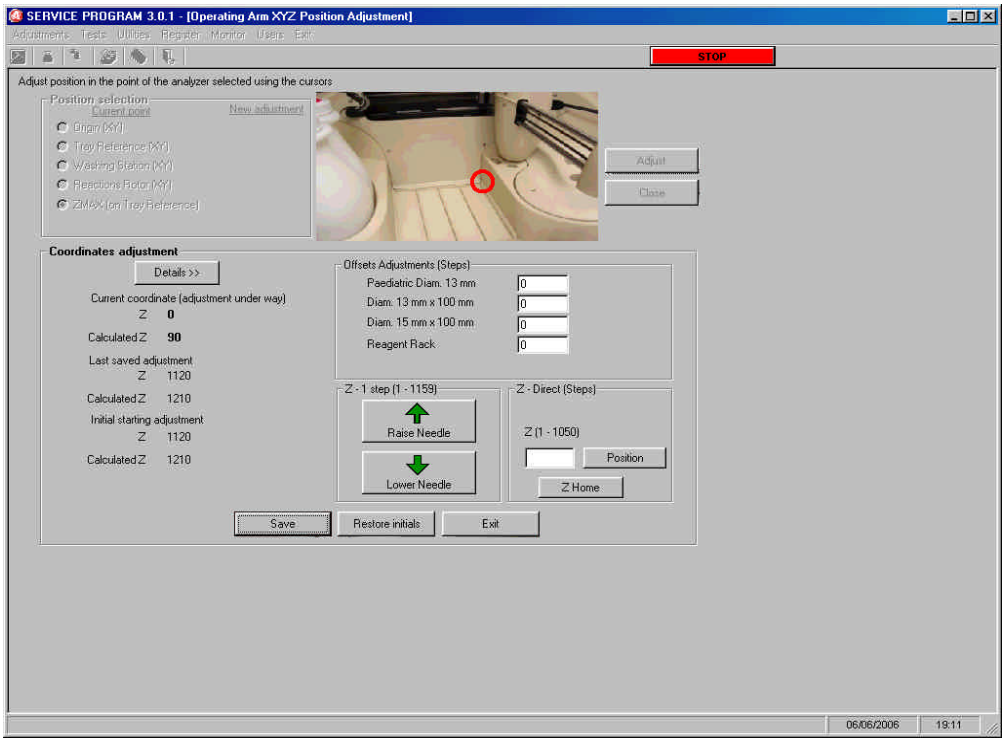

reinitialise the Z axis and repeat the process from the beginning.

- Part 2 adjusts the offsets to reduce the zero volume without colliding with the racks, adding or subtracting steps to or from the value adjusted in part 1. This operation must be carried out by trial and error. First enter a low step value for the type of rack and then proceed to the Zmax verification motor test. Indicate the type of rack and position on the tray. Position the rack with the bottles and the primary or paediatric wells, as applicable. Perform the test and check whether the needle is far from or collides with the bottom. As necessary, return to the Zmax adjustment menu and increase or decrease the step value on the offset that corresponds to the rack type. Remember that if the needle collides with the bottom during the test, it retreats a few steps since encoder detection is not enabled.

4.2.4. Adjustment of the positioning of the rotor

This screen enables the adjustment of the positioning of the rotor with regard to the dispensing point and the optical system. One or the other is selected by means of two different tabs.

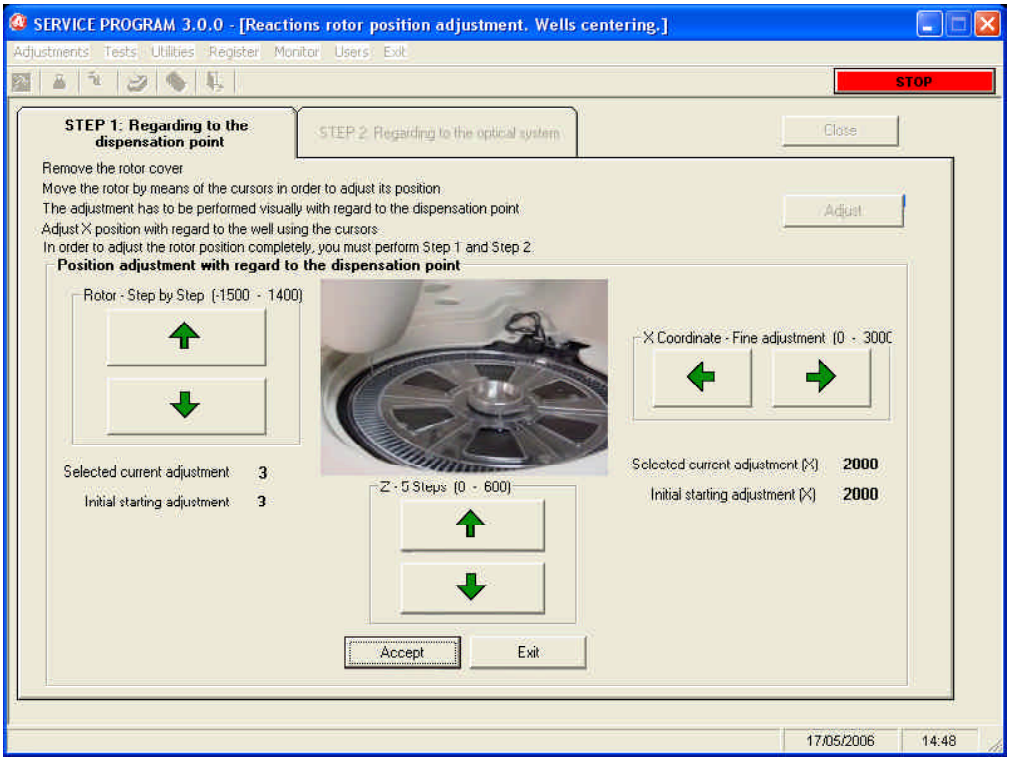
SERVICE PROGRAM 3.0.0 - [Reactions rotor position adjustment. Wells centering.]
Adjustments
Tests
Utilities
Register
Monitor
Users
Exit
STOP
STEP 1: Regarding to the dispensation point
STEP 2: Regarding to the optical system
Close
Remove the rotor cover
Move the rotor by means of the cursors in order to adjust its position
The adjustment has to be performed visually with regard to the dispensation point
Adjust X position with regard to the well using the cursors
In order to adjust the rotor position completely, you must perform Step 1 and Step 2
Adjust
Position adjustment with regard to the dispensation point
Rotor - Step by Step (-1500 - 1400)
X Coordinate - Fine adjustment (0 - 3000
Selected current adjustment 3
Initial starting adjustment 3
Selected current adjustment (X) 2000
Initial starting adjustment (X) 2000
Z - 5 Steps (0 - 600)
Accept
Exit
17/05/2006
14:48

4.2.4.1. Centering of the rotor with regard to the dispensing point

The analyzer initialises the rotor and positions the first rotor well at the currently programd dispensing position. The technician has buttons to move the rotor step by step to adjust, if necessary, this position and buttons for finer adjustment of the X coordinate over the dispensing point. At all times, the screen shows the current dispensing coordinate on the first well and of the X axis position, the last coordinate stored and the initial screen input coordinate, as additional information for the technician. When this is satisfactory, the current coordinate of the dispensing point of the first well can be stored by pressing the *Store* button. Pressing the *Cancel* button keeps the last stored value and the current value is not stored. Pressing the *Restore* button restores the initial screen input value.

4.2.4.2. Centering of the rotor with regard to the optical system

This adjustment is necessary only if the *Rotor Centering Adjustment* has been carried out with regard to the dispensing point (4.1.4.1.). This adjustment must be made with the rotor cover in position. The analyzer initialises the rotor and fills the first 3 wells of the rotor with distilled water. Next, step-by-step optical readings are made through these wells at the wavelength selected by the technician. Once the readings have ended, the program shows a graph of the light intensity measured on the rotor steps. On this graph, the program indicates at which

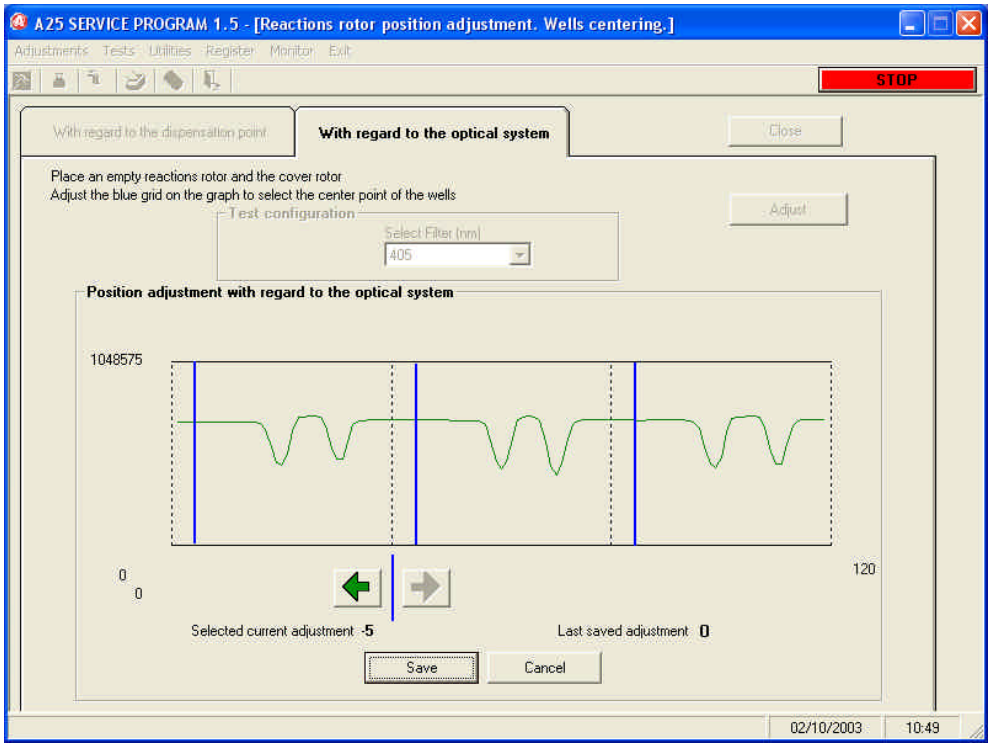

points the optical readings are made on each of the 3 wells when the analysis is made, with the coordinate of the reading point of the first well currently programd in the analyzer. If necessary, the technician can move the reading points over the graph jointly using two buttons. The optimum reading point is that which globally maximises the light intensity for the three wells. At all times, the screen shows the current coordinate of the reading in the first well and the last coordinate stored, as additional information for the technician. When the position is satisfactory, the current coordinate of the reading point of the first well can be stored by pressing the *Store* button. Pressing the *Cancel* button keeps the last stored value and the current value is not stored.

4.2.5 . Adjustment of the positioning of the filter wheel

This adjustment must be made with the rotor cover in position. The analyzer initialises the rotor and the filter wheel and fills the first rotor well with distilled water. Next, it takes optical readings through this well, turning the filter

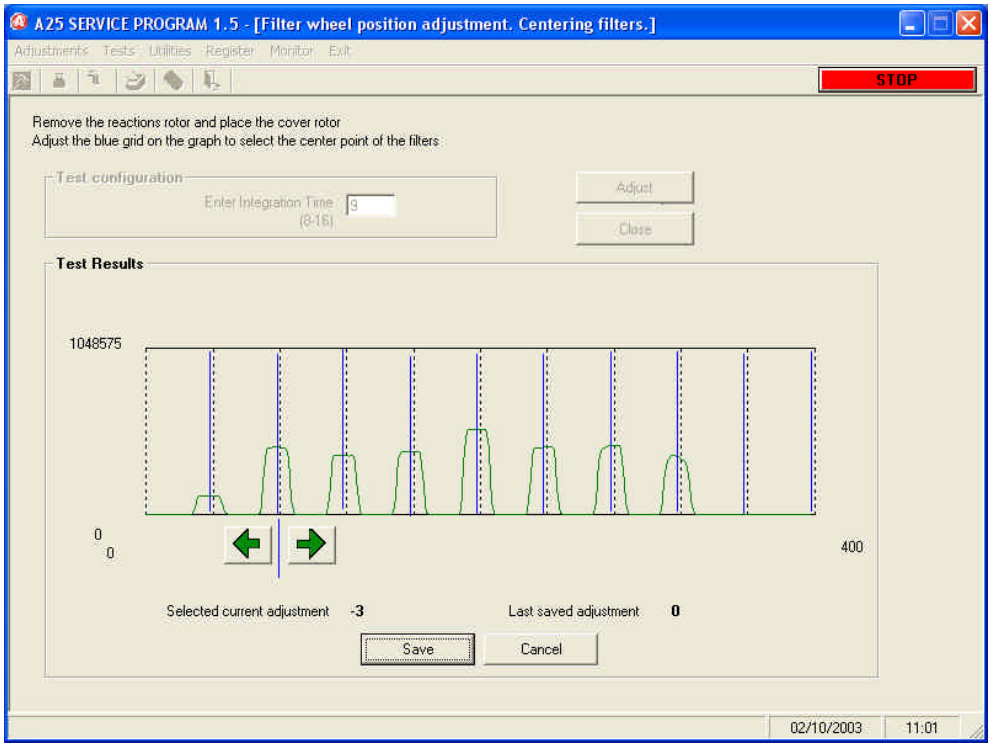

wheel step by step, with a certain integration time as indicated by the technician (the concept of *integration time* is explained in the section on photometric adjustments). Once the readings have ended, the program shows a graph of the light intensity measured on the steps of the filter wheel. On this graph, the program indicates at which points each of the filters is positioned when optical readings are taken when the analysis is carried out, with the coordinate of the positioning of the filter 0 currently programd in the analyzer. If necessary, the technician can move the reading points over the graph jointly using two buttons. The optimum reading point is that which globally maximises the light intensity for all the filters. At all times, the screen shows the current coordinate of the filter 0 and the last coordinate stored, as additional information for the technician. When the position is satisfactory, the current coordinate of the positioning of the filter 0 can be stored by pressing the *Store* button. Pressing the *Cancel* button keeps the last stored value and the current value is not stored.

4.2.6. Adjustment of the level control scales

This screen makes it possible to set the level control scales with the empty waste and distilled water containers (0% capacity) and when they are full (100% capacity). The maximum capacity of the containers is approximately

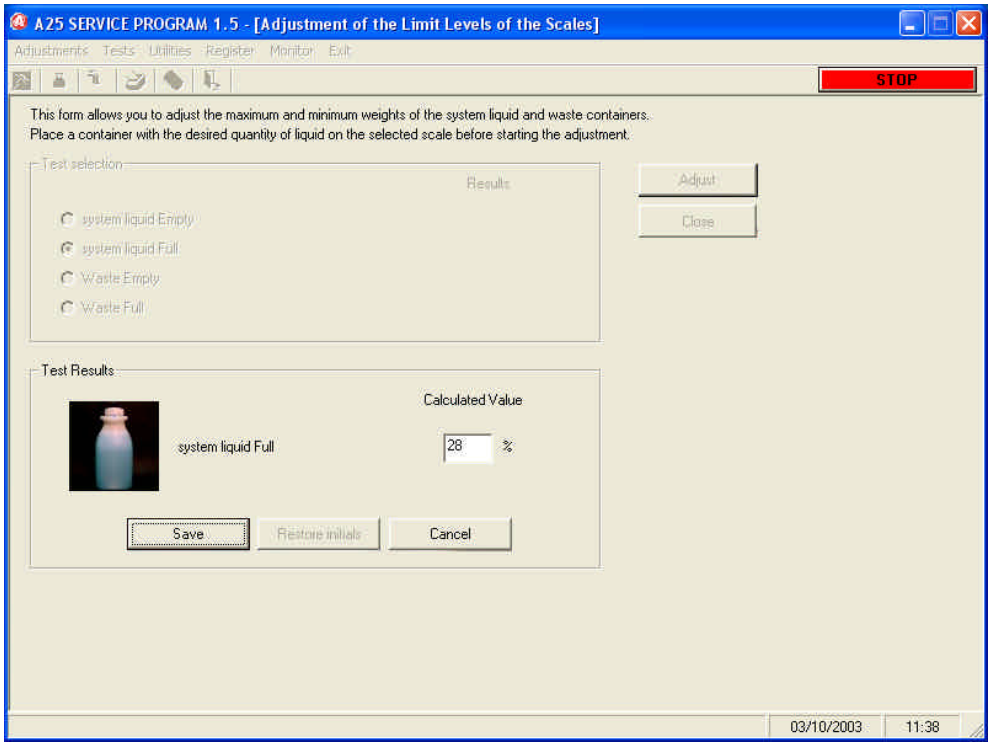

3L. The technician must choose whether he wishes to set the distilled water or waste container scales, with the corresponding container full or empty. According to the requested adjustment, the corresponding container, full or empty, must be placed in position and the *Adjust* button pressed. Based on the settings made, the analyzer automatically adjusts the scales. On pressing the *Store* button, the analyzer saves the new values of the adjusted parameters. Pressing the *Cancel* button keeps the last stored values and the current values are not stored.

4.2.7. Adjustment of the level detection sensitivity

This screen allows fitting the sensitivity of the capacity level detection system of the probe. In order to make the adjustment, first of all you have to select a rack and place on it the following configuration of racks and samples:

- Paediatric Rack: place 4 paediatric glasses in positions 5, 6, 17 and 18 with 300 uL of distilled water.
- Rack of 13/15mm sample: place 4 tubes in positions 5, 6, 17 and 18 with 300 uL of distilled water.
- Rack of reagents: place 2 bottles of 20mL in positions 5 and 6 with 2mL of distilled water.

It is possible to see a graphic with the position of the tubes and racks in the screen photo. When pressing the Adjust button, the arm takes some sensitivity readings automatically until detecting the water in each one of the tubes. Once this operation is finished, the arm is parked in its original position and it shows the sensitivity results

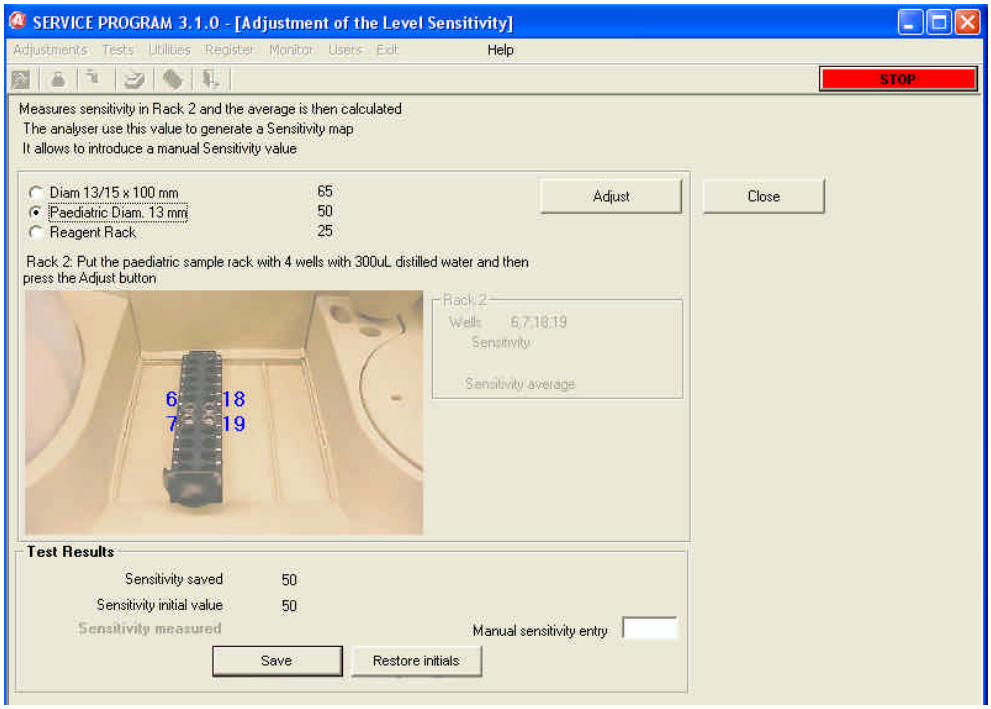
SERVICE PROGRAM 3.1.0 - [Adjustment of the Level Sensitivity]
Adjustments Tests Utilities Register Monitor Users Exit
Help
STOP
Measures sensitivity in Rack 2 and the average is then calculated
The analyser use this value to generate a Sensitivity map
It allows to introduce a manual Sensitivity value
Diam 13/15 x 100 mm 65
Paediatric Diam. 13 mm 50
Reagent Rack 25
Adjust
Close
Rack 2: Put the paediatric sample rack with 4 wells with 300uL distilled water and then press the Adjust button
Rack 2
Wells 6,7,18,19
Sensitivity
Sensitivity average
Test Results
Sensitivity saved 50
Sensitivity initial value 50
Sensitivity measured
Manual sensitivity entry
Save
Restore initials

of each one of the tubes. Move rack to position 5 and repeat the adjustment. Once these second readings are finished, the program calculates the average of all sensitivities; the result is the average sensitivity. The technician should notice that the sensitivity values of each tube have to be similar; otherwise, he should repeat the whole measurement.
Repeat this adjustment per each rack type.
The sensitivity value can also be introduced manually for each rack in the corresponding box.

Pressing the button Save, the analyser saves the new adjusted sensitivity value. Pressing the button Close, the old value stays. Pressing the button Restore, the initial value of entry to the screen is restored. A manual sensitivity value can be inserted in the corresponding box.

4.3. TESTS

Various tests make it possible to check that the different components of the analyzer function correctly.

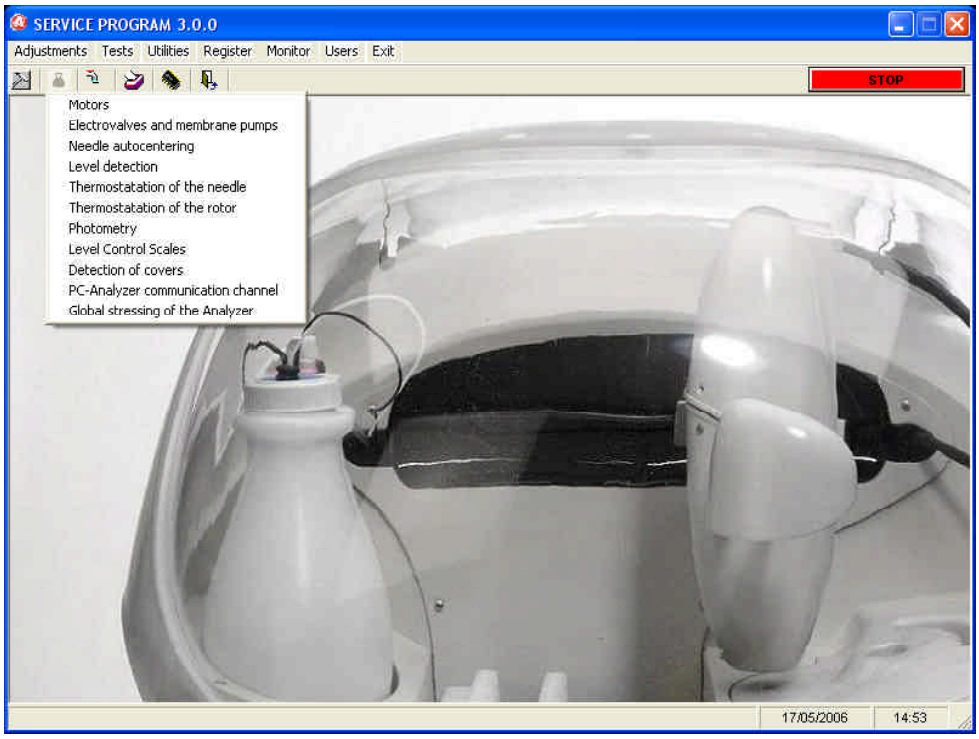

4.3.1. Motor tests

Through these tests, the technician can check the correct functioning of all the analyzer motors step by step. The screen makes it possible to choose the motor to be tested and the test that is to be carried out. The analyzer uses the following motors step by step:
- X axis of the operating arm.
- Y axis of the operating arm.
- Z axis of the operating arm.
- Dispensing pump
- Rotor
- Filter wheel

All the motor tests can be performed without the covers and housing of the analyzer. After the verifications, the operating arm always returns to its resting position. To test the motor of the dispensing pump, the arm is positioned over the washing station. It is convenient for the dispensing system to be primed so that the piston does not function dry. The following is a description of the different tests that can be performed.

4.3.1.1. Initialization test

This test verifies the start detector of each of the motors.

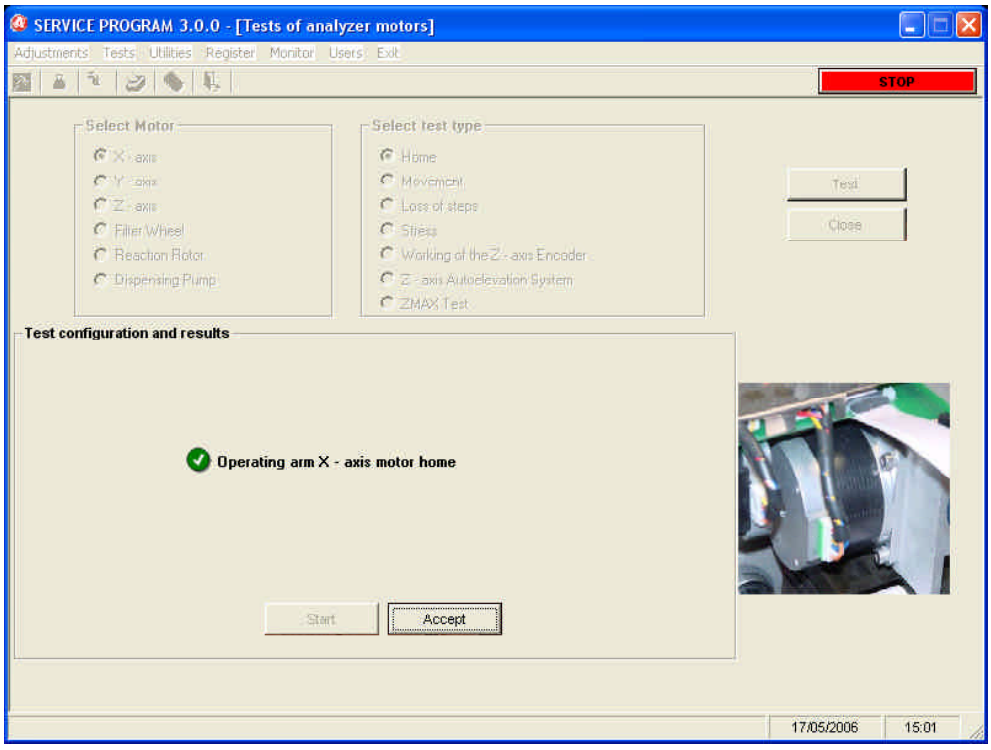

4.3.1.2. Movement test

This test displaces any of the mobile components to the desired point along its range of functioning, introducing the corresponding absolute coordinate or moving it step by step. The speed and acceleration of the movement are those used in the normal functioning of the analyzer.

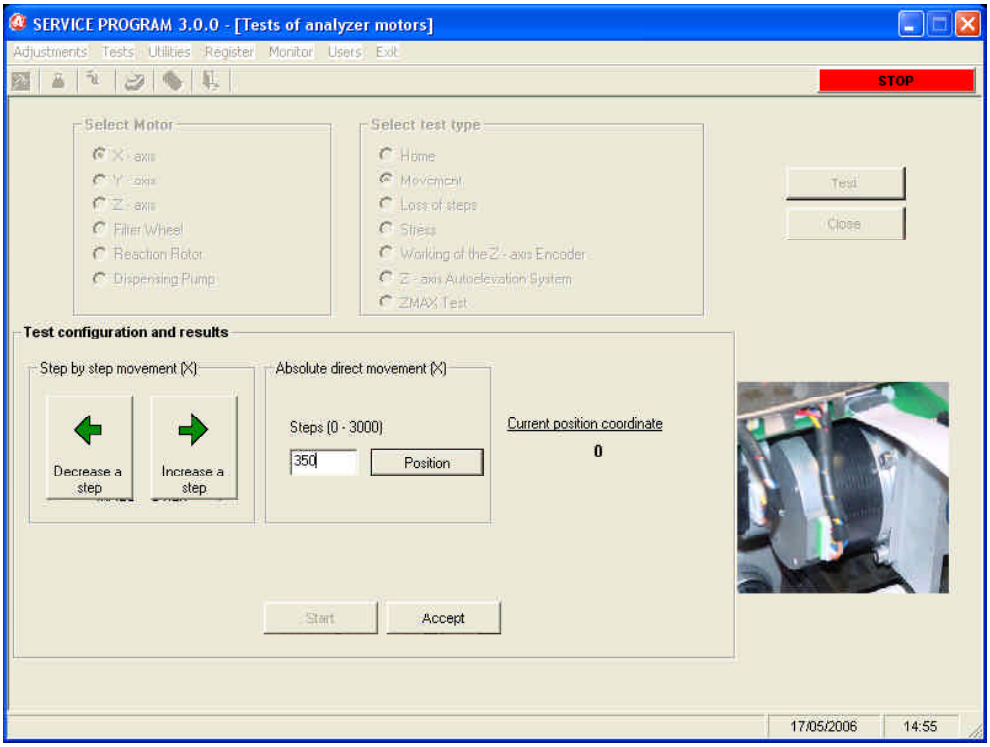

4.3.1.3. Loss step test

This test makes it possible to check if a motor misses steps when performing a certain sequence of movements. The test can be carried out with the speed and acceleration used in the normal functioning of the analyzer or with these magnitudes increased by 10% to check the functioning safety margin.

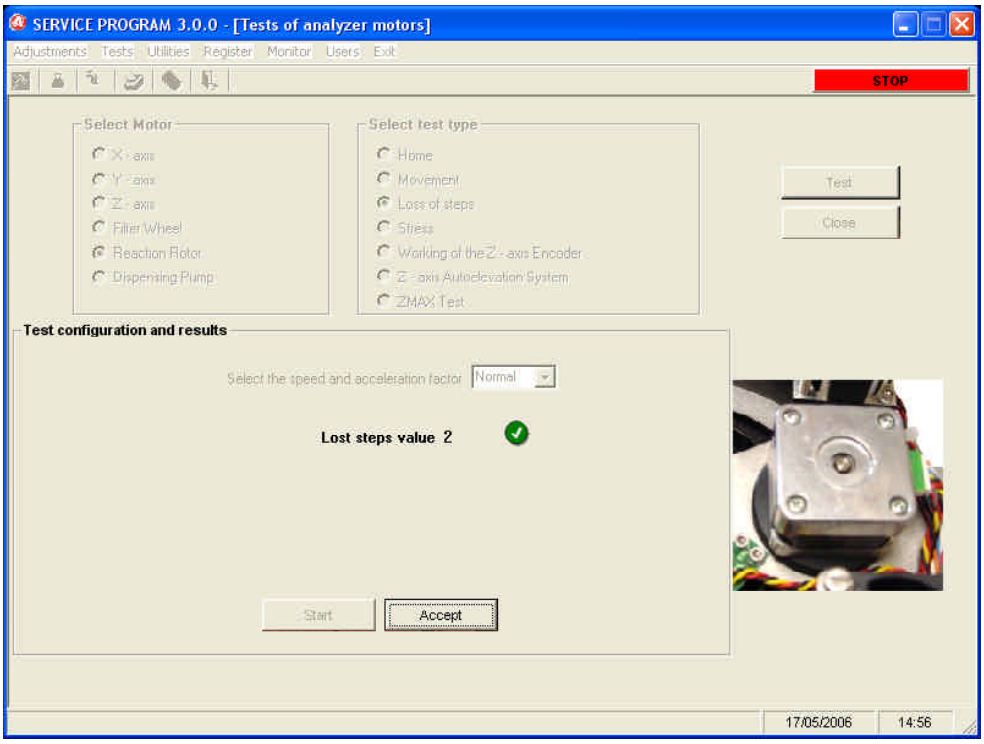

4.3.1.4. Stress mode test

This test makes it possible for a certain sequence of movements to be performed continually. The technician can program the duration of the test, which can be cancelled at any moment. Depending on the motor selected, there is a minimum stress mode time (but in no case is it higher than 50 seconds).

4.3.1.5. Z axis security systems test

The Z axis of the operating arm has an encoder to detect if there have been missed steps as a result of a collision with the needle. In the case of a power failure, a mechanical system automatically raises the needle. On selecting the corresponding options, the analyzer checks the functioning of each of these devices.

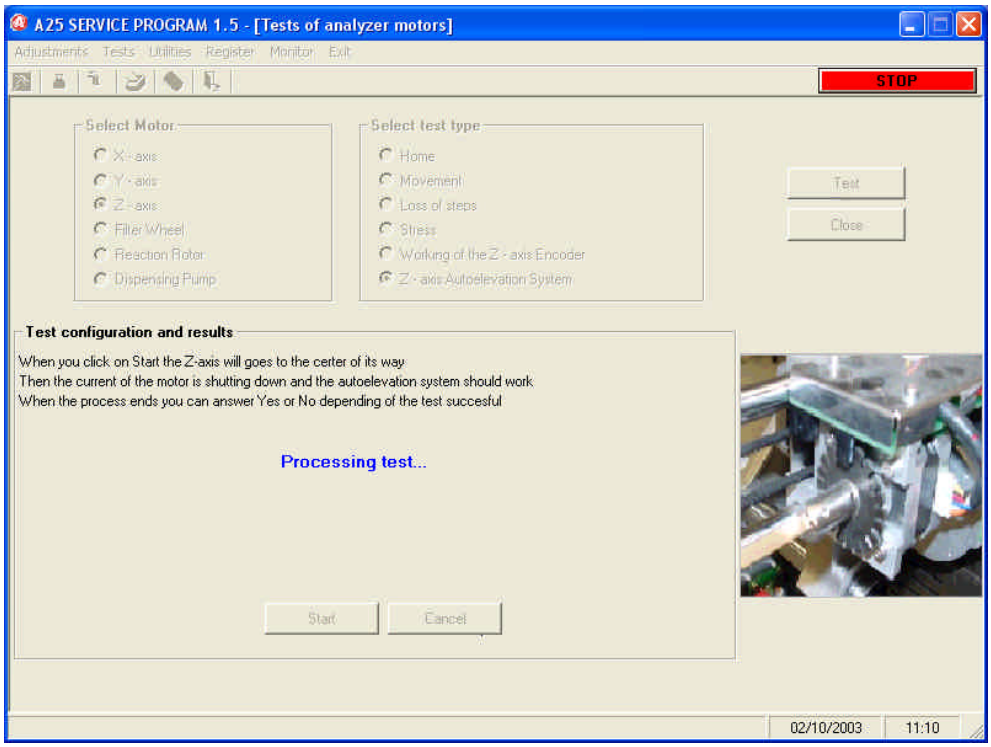
A25 SERVICE PROGRAM 1.5 - [Tests of analyzer motors]
Adjustments Tests Utilities Register Monitor Exit
STOP
Select Motor
X - axis
Y - axis
Z - axis
Filter Wheel
Reaction Rotor
Dispensing Pump
Select test type
Home
Movement
Loss of steps
Stress
Working of the Z - axis Encoder
Z - axis Autoelevation System
Test
Close
Test configuration and results
When you click on Start the Z-axis will goes to the certer of its way
Then the current of the motor is shutting down and the autoelevation system should work
When the process ends you can answer Yes or No depending of the test succesful
Processing test...
Start
Cancel
02/10/2003
11:10

4.3.1.6 Maximum Z verification test

This test checks that the needle does not collide with the bottles on the rack tray. Select the rack type (reagent, paediatric, 30 mm or 15 mm), the position of the rack on the tray and the position of the bottle or well on the rack. Press the *Start* button to move to the selected position and check if the needle collides with the bottle or well or if there is space between the needle and the bottle.
Repeat the process in the positions required by the user.

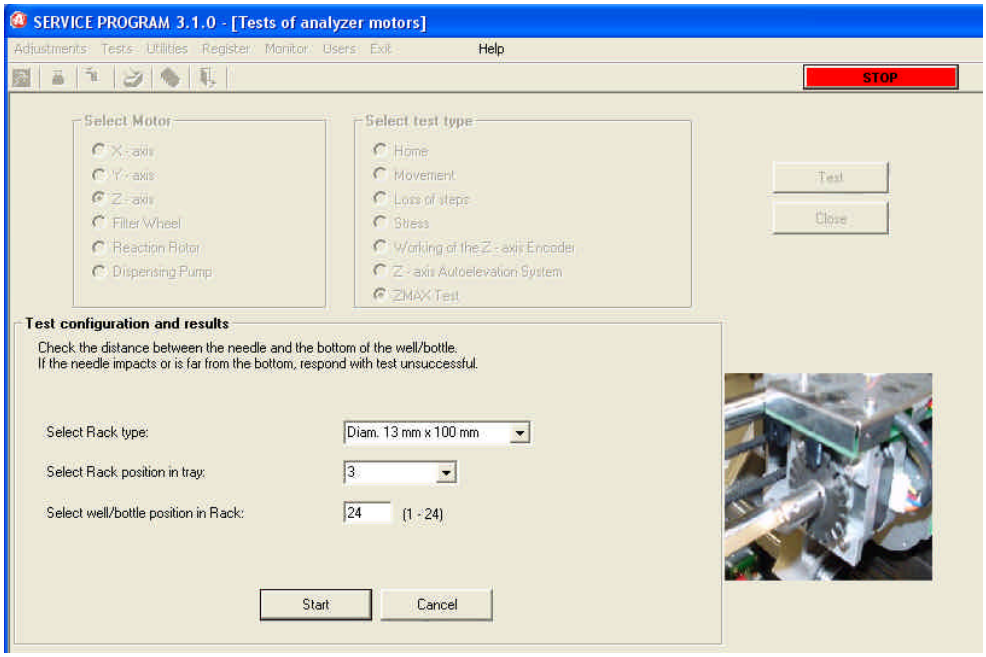

4.3.2. Diaphragm pumps and electrovalves test

The analyzer uses a 3-way electrovalve to manage the dispensing operations. The washing system of the needle uses a 2-way electrovalve and two diaphragm pumps. The screen makes it possible to choose the device to be tested and the test that is to be carried out. The devices that can be tested independently are:

- 3-channel electrovalve of the dispensing pump.
- 2-channel electrovalve of the washing system.
- Washing system diaphragm pumps

To carry out these tests, the dispensing system should be primed. The following is a description of the different tests that can be performed.

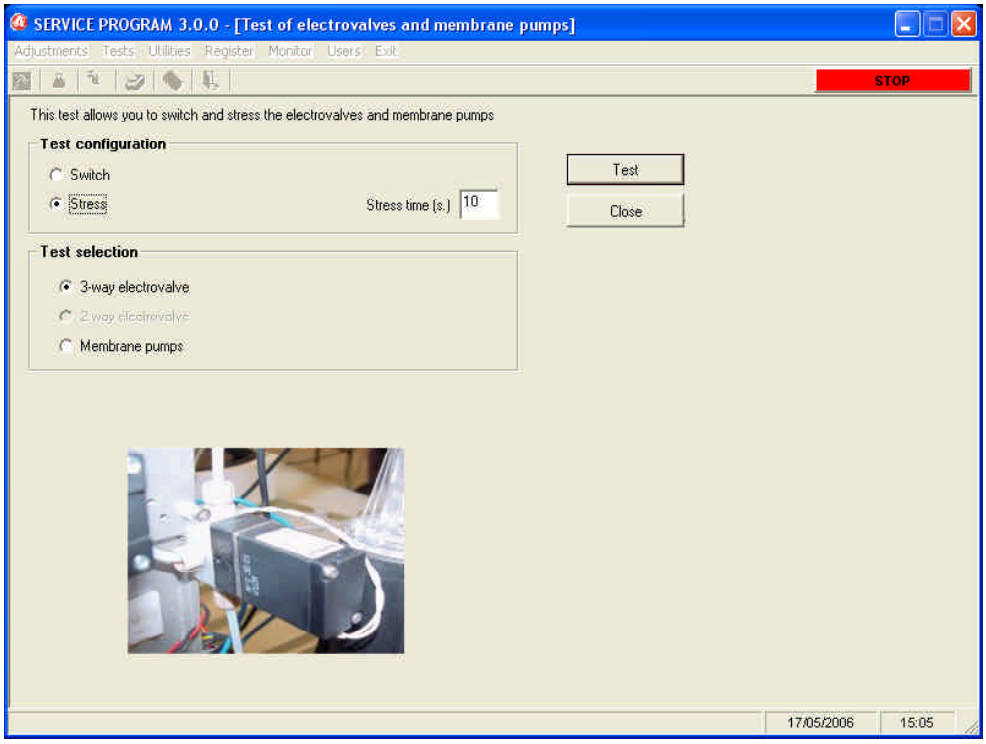

4.3.2.1. Functioning test

This test makes it possible to manually switch the selected device.

4.3.2.2. Stress mode test

This test makes it possible for a certain sequence of device switching to be performed continually. The technician can program the duration of the test, which can be cancelled at any moment.

4.3.3. Needle self-centering system test

This test makes it possible to check the functioning of the needle self-centering system. During its initialisation, the analyzer uses this system to check the presence of the needle and its verticality and automatically correct small deviations. The test consists of simply running this process. The technician can remove the housing of the arm to observe the test. On the finalisation of the test, the program shows the deviation (x, y) found in the motor steps.

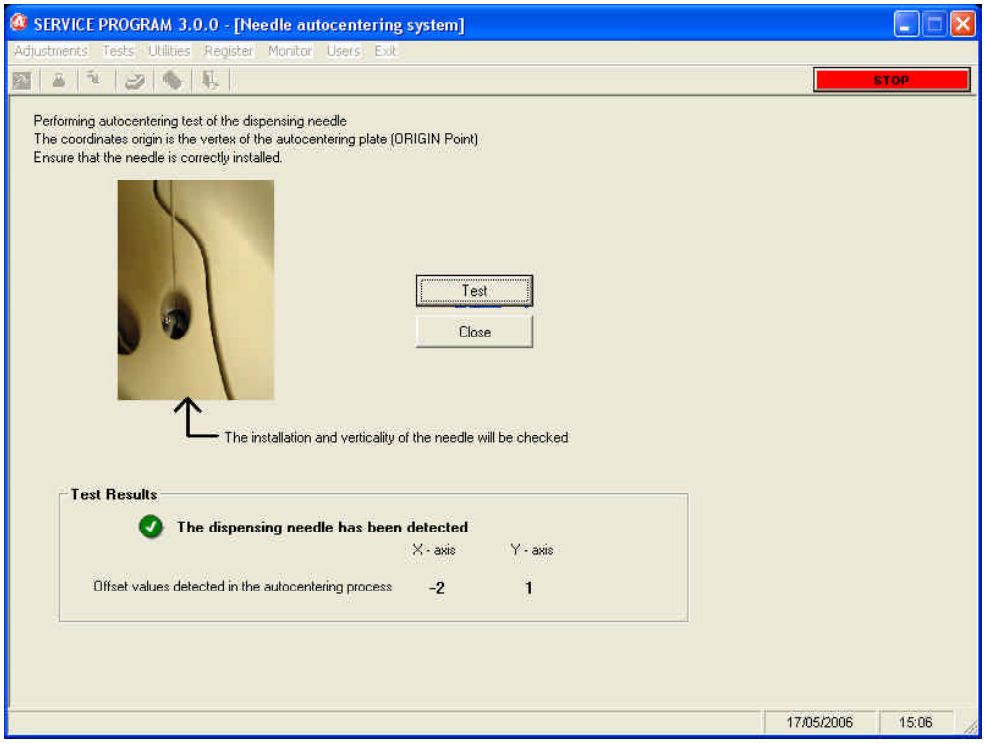
SERVICE PROGRAM 3.0.0 - [Needle autocentering system]
Adjustments Tests Utilities Register Monitor Users Exit
STOP
Performing autocentering test of the dispensing needle
The coordinates origin is the vertex of the autocentering plate (ORIGIN Point)
Ensure that the needle is correctly installed.
Test
Close
The installation and verticality of the needle will be checked
Test Results
The dispensing needle has been detected
X - axis
Y - axis
Offset values detected in the autocentering process
-2
1
17/05/2006
15:06

4.3.4. Needle level detection system test

This test checks the functioning of the system for detecting the capacity of the needle in bottles of reagent and sample tubes.
This test checks the functioning of the system for detecting the capacity of the needle in reagent bottles and sample wells. The test can be performed in any position on the tray.
First select the rack type, then the position of the rack on the tray and, finally, the position of the bottle/well on the rack. Press the *Test* button and the program will move the arm to the indicated position and check whether or not liquid is detected, depending on whether the bottle is full or empty.
Repeat the test as many times as the user considers necessary.

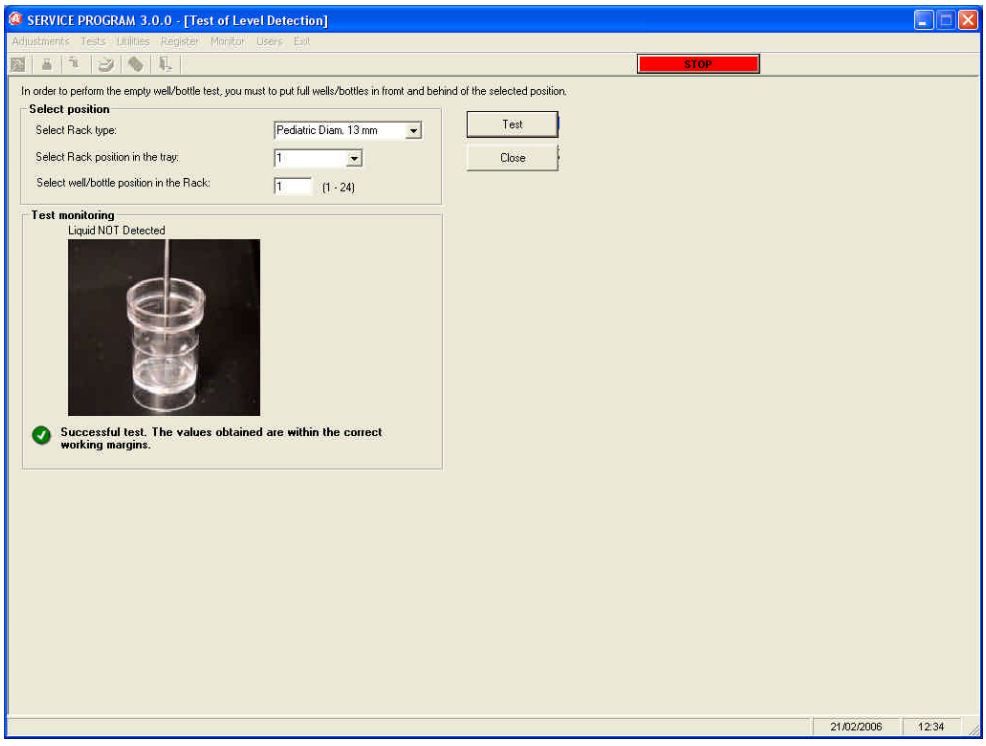
SERVICE PROGRAM 3.0.0 - [Test of Level Detection]
Adjustments Tests Utilities Register Monitor Users Exit
STOP
In order to perform the empty well/bottle test, you must to put full wells/bottles in front and behind of the selected position.
Select position
Select Rack type:
Pediatric Diam. 13 mm
Select Rack position in the tray:
1
Select well/bottle position in the Rack:
1
(1 - 24)
Test
Close
Test monitoring
Liquid NOT Detected
Successful test. The values obtained are within the correct working margins.
21/02/2006
12:34

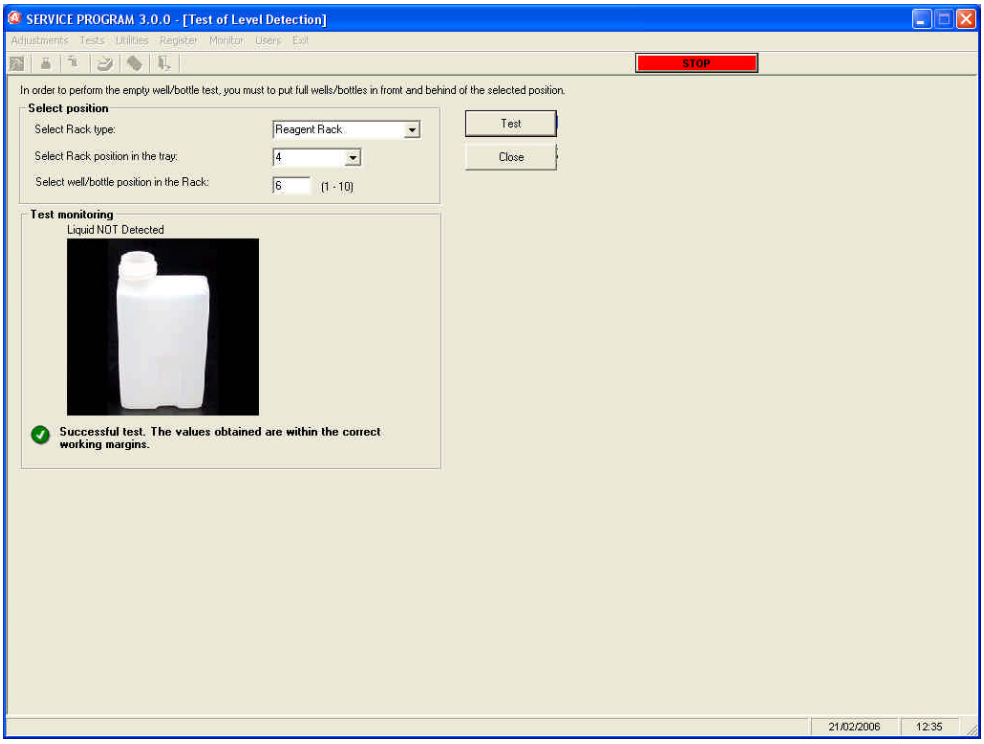
SERVICE PROGRAM 3.0.0 - [Test of Level Detection]
Adjustments Tests Utilities Register Monitor Users Exit
STOP
In order to perform the empty well/bottle test, you must to put full wells/bottles in fromt and behind of the selected position.
Select position
Select Rack type:
Reagent Rack
Select Rack position in the tray:
4
Select well/bottle position in the Rack:
6
(1 - 10)
Test
Close
Test monitoring
Liquid NOT Detected
Successful test. The values obtained are within the correct working margins.
21/02/2006
12:35

4.3.5. Needle thermostatation system test

This screen makes it possible to check that the dispensing temperature of the reactions is around 37ºC. To make this adjustment, the analyzer must be initialised. The technician must measure the temperature of the dispensed liquid with a thermometer calibrated at 37ºC. The program shows the set point temperature of the current control. This parameter must be different from 37ºC. When the technician so indicates, the analyzer dispenses thermostated distilled water on a certain position in the racks tray shown on the screen. The technician must measure the temperature of the water with the calibrated thermometer and introduce the temperature on the screen. The program indicates if the temperature measured is within the tolerated error margins and stores this value for the test result reports. The liquid to be dispensed is taken from the system liquid container or from the bottle of reagent selected by the technician.

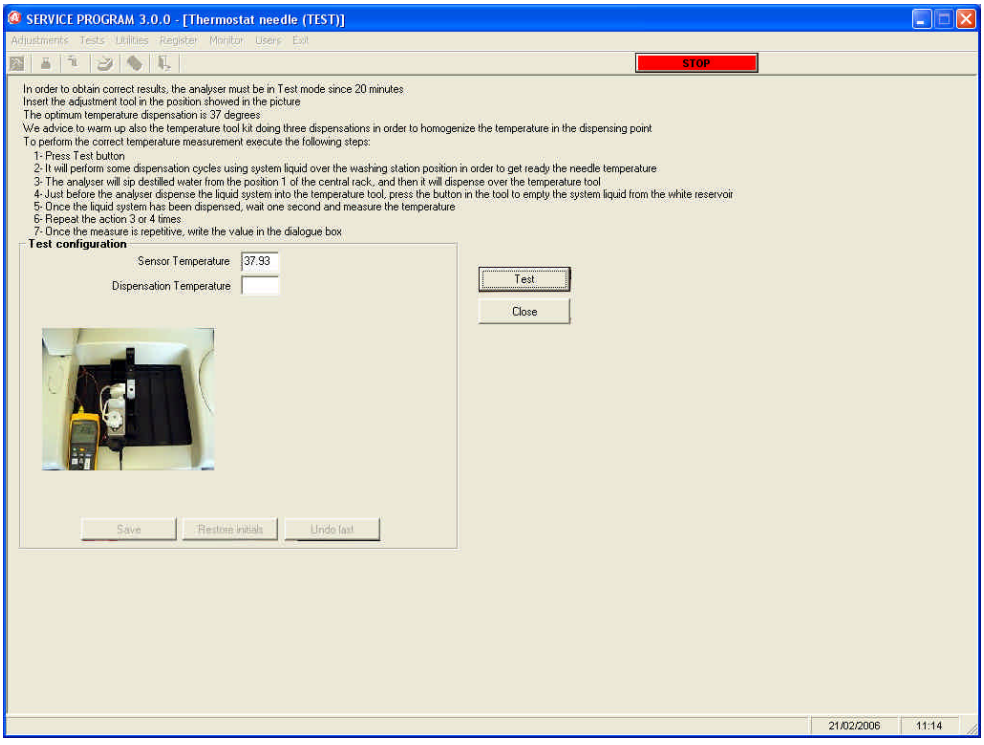
SERVICE PROGRAM 3.0.0 - [Thermostat needle (TEST)]
Adjustments Tests Utilities Register Monitor Users Exit
STOP
In order to obtain correct results, the analyser must be in Test mode since 20 minutes
Insert the adjustment tool in the position showed in the picture
The optimum temperature dispensation is 37 degrees
We advice to warm up also the temperature tool kit doing three dispensations in order to homogenize the temperature in the dispensing point
To perform the correct temperature measurement execute the following steps:
1- Press Test button
2- It will perform some dispensation cycles using system liquid over the washing station position in order to get ready the needle temperature
3- The analyser will sip destilled water from the position 1 of the central rack., and then it will dispense over the temperature tool
4- Just before the analyser dispense the liquid system into the temperature tool, press the button in the tool to empty the system liquid from the white reservoir
5- Once the liquid system has been dispensed, wait one second and measure the temperature
6- Repeat the action 3 or 4 times
7- Once the measure is repetitive, write the value in the dialogue box
Test configuration
Sensor Temperature
37.93
Dispensation Temperature
Test
Close
Save
Restore initials
Undo last
21/02/2006
11:14

4.3.6. Needle rotor thermostatation system test

This screen makes it possible to check that the temperature of the rotor reactions is 37ºC. To make this test, the analyzer must be initialised. The methacrylate rotor can be automatically filled with distilled water by pressing the corresponding button. Once filled, the technician must wait a few minutes for the rotor to be thermostated. The temperature in the rotor wells must be measured with a temperature calibrated at 37ºC through the dispensing hole of the rotor cover. A button makes it possible to turn the rotor in increases of 15 wells to change the well on which the measurement is being taken. The program shows the set point temperature of the current control. This parameter must be other than 37ºC. The technician must measure the temperature of the water with the calibrated thermometer in the wells and enter the temperature on the screen. The program indicates if the temperature measured is within the tolerated error margins and stores this value for the test result reports.

SERVICE PROGRAM 3.0.0 - [Rotor Thermostatation (TEST)]
Adjustments
Tests
Utilities
Register
Monitor
Users
Exit
STOP
REMEMBER: You must have performed the Warming Up for the measurements to be significant.
After filling the rotor, wait 5 to 10 minutes for the liquid to reach its final temperature.
You must wait every time the sensor temperature is modified.
To check the homogeneity of the temperature inside the rotor, measurements have to be made in the different positions.
The final result is calculated from the average of all the wells temperatures measured. The optimum temperature of the liquids is 37 degrees
Due to the structure of the reactions rotor, the measurement in position 1 is lower. The Analyzer corrects it automaticly.
Rotor filling
Insert a manually filled rotor
Automatic rotor filling by the analyzer
Apply
Test configuration
Sensor temperature
38.43
Average measured temperature
Rotor measurement position
1
Do Measurement
Test
Close
Save
Restore initials
Undo last
Before measuring, wait from 5 to 10 minutes for the liquid in the rotor to reach an estable temperature
17/05/2006
15:32

4.3.7. Photometry tests

This screen contains a set of tests to check the functioning of the optical system. The tests are classified under different tabs. First of all, the base line and darkness count tests must be made in order to be able to carry out the remaining tests. To perform these tests, the analyzer must be initialised.

The optical system has a photodiode that generates an electrical current proportionate to the light intensity on it. *time*. An AD converter converts the accumulated load into a digital value called *count number*, between 0 and 1048576. During normal functioning, the analyzer automatically adjusts the integration time for each filter when the analysis begins and after initialisation. When the first photometry test is performed, the integration times are also automatically adjusted. These times are adjusted in such a way that the count number of the base line for each wavelength is as near as possible to 950000. In this way, the dynamic range of the detection system is adapted to the light intensity present at each wavelength. The filter wheel has 10 positions. Position 0 must always contain a covered filter so that the analyzer can perform the darkness adjustment. Positions 1 to 9 can be used for optical filters.

4.3.7.1. Base line and integration times

When this test is run for the first time, the analyzer fills the first 3 rotor wells with distilled water. The analyzer automatically adjusts the integration times and makes a base line with each of the available filters in each of the 3 wells. The program shows the current integration times for each of the filters and the average for the 3 wells of the

count numbers obtained with each filter. The screen shows the corresponding alarms in the case of anomaly. It is also possible to access a screen where it is possible to manually vary the integration times to check their effect on the count numbers. And another screen where it is possible to assign calculated integration times as reference integration times for each filter. This screen is recommended when a filter or the lamp is physically changed. After performing the test, the analyzer continues to take optical readings using the automatically adjusted integration times.

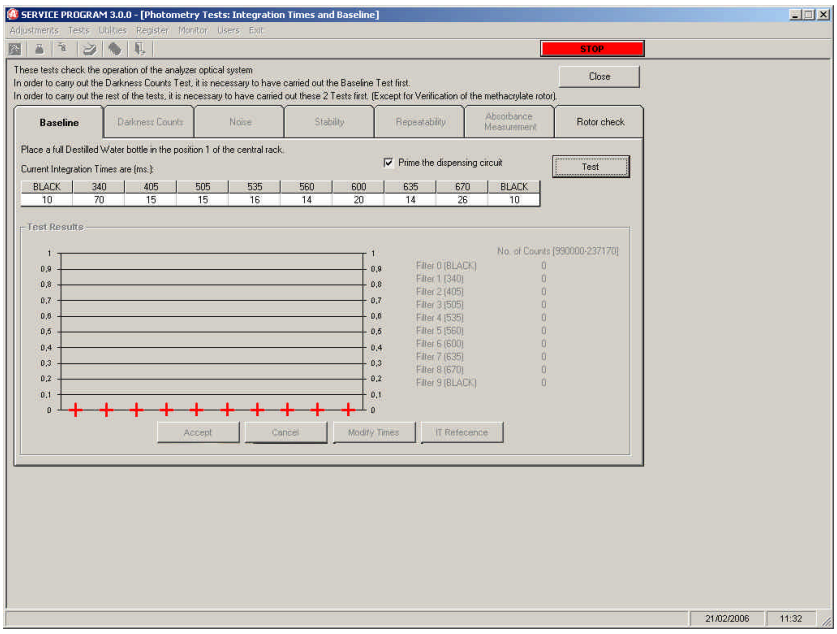

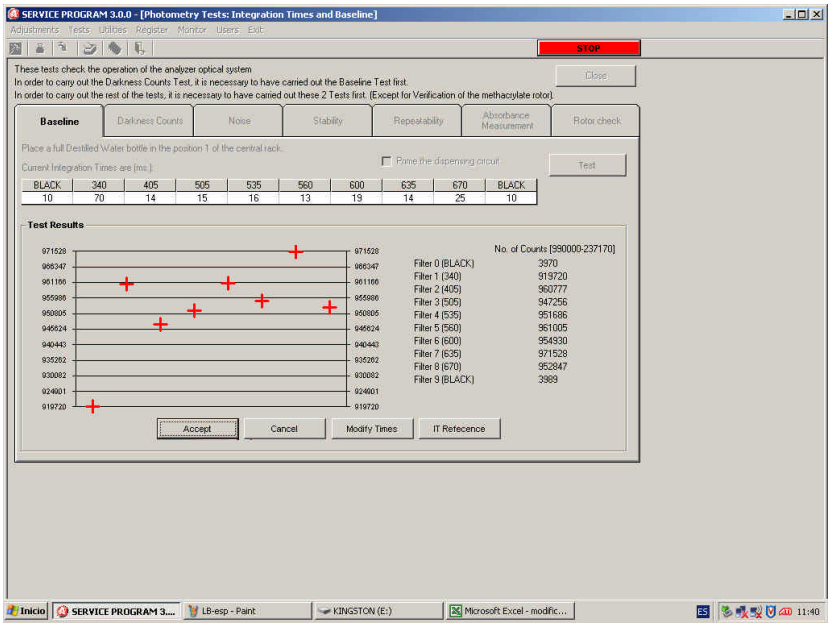

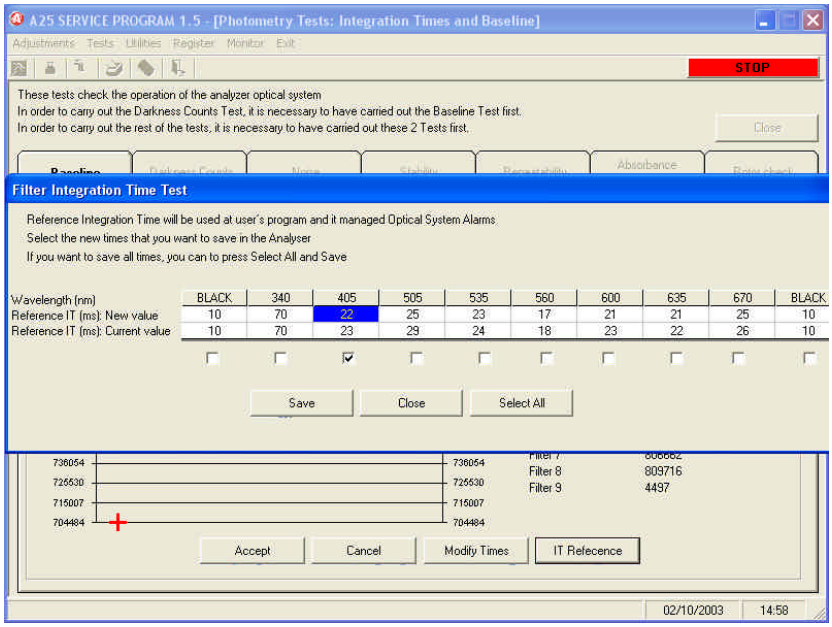
A25 SERVICE PROGRAM 1.5 - [Photometry Tests: Integration Times and Baseline]
Adjustments Tests Utilities Register Monitor Exit
STOP
These tests check the operation of the analyzer optical system
In order to carry out the Darkness Counts Test, it is necessary to have carried out the Baseline Test first.
In order to carry out the rest of the tests, it is necessary to have carried out these 2 Tests first.
Close
Absorbance
Filter Integration Time Test
Reference Integration Time will be used at user's program and it managed Optical System Alarms
Select the new times that you want to save in the Analyser
If you want to save all times, you can to press Select All and Save
Wavelength (nm) BLACK 340 405 505 535 560 600 635 670 BLACK
Reference IT (ms): New value 10 70 22 25 23 17 21 21 25 10
Reference IT (ms): Current value 10 70 23 29 24 18 23 22 26 10
Save
Close
Select All
736054
726530
715007
704484
Filter 8 809716
Filter 9 4497
Accept
Cancel
Modify Times
IT Refecence
02/10/2003
14:58

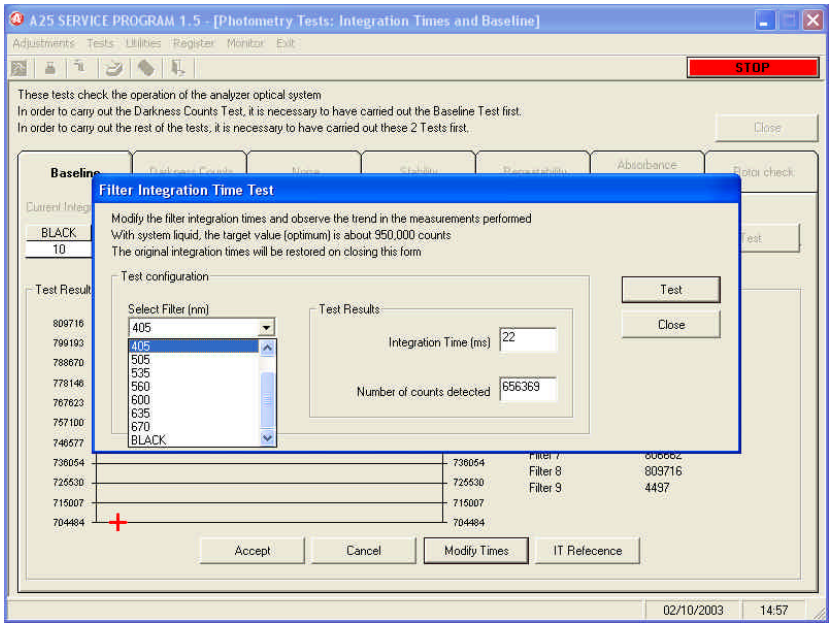
A25 SERVICE PROGRAM 1.5 - [Photometry Tests: Integration Times and Baseline]
STOP
These tests check the operation of the analyzer optical system
In order to carry out the Darkness Counts Test, it is necessary to have carried out the Baseline Test first.
In order to carry out the rest of the tests, it is necessary to have carried out these 2 Tests first.
Close
Baseline
Absorbance
Rotor check
Filter Integration Time Test
Modify the filter integration times and observe the trend in the measurements performed
With system liquid, the target value (optimum) is about 950,000 counts
The original integration times will be restored on closing this form
Test configuration
Select Filter (nm)
405
505
535
560
600
635
670
BLACK
Test Results
Integration Time (ms) 22
Number of counts detected 656369
Test
Close
Filter 8 809716
Filter 9 4497
Accept
Cancel
Modify Times
IT Refecence
02/10/2003
14:57

4.3.7.2. Darkness counts

The program shows the current integration times for each filter. On running the test, the analyzer positions the covered filter and measures the darkness counts with each of the integration times. Each time an optical reading is taken, the analyzer subtracts these darkness counts from the count numbers measured to obtain the light intensity. The program shows the values obtained and issues the corresponding alarms in case of anomaly. The values should be around 4100 - 4300. All the count numbers shown by the tests given as follows have the darkness counts subtracted.

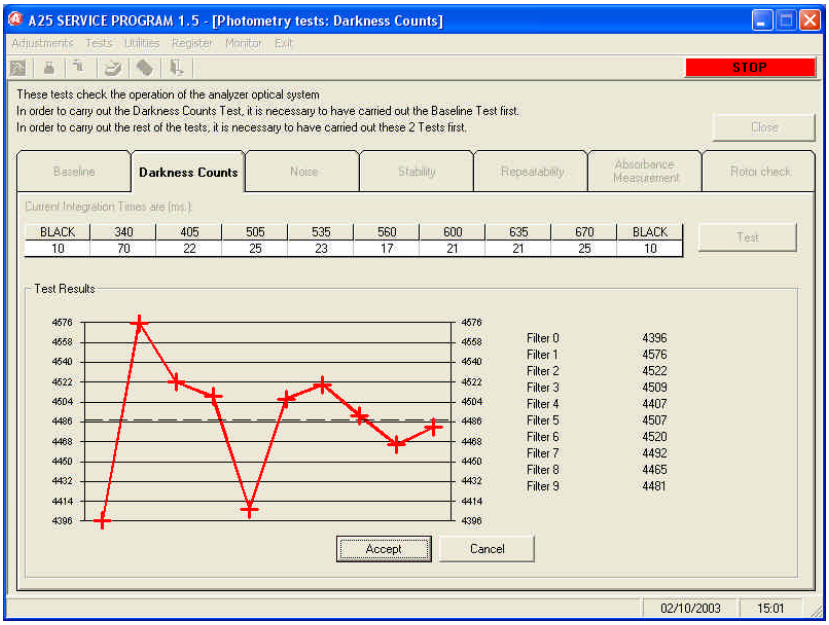
A25 SERVICE PROGRAM 1.5 - [Photometry tests: Darkness Counts]
Adjustments Tests Utilities Register Monitor Exit
STOP
These tests check the operation of the analyzer optical system
In order to carry out the Darkness Counts Test, it is necessary to have carried out the Baseline Test first.
In order to carry out the rest of the tests, it is necessary to have carried out these 2 Tests first.
Close
Baseline
Darkness Counts
Noise
Stability
Repeatability
Absorbance Measurement
Rotor check
Current Integration Times are (ms.):
BLACK 340 405 505 535 560 600 635 670 BLACK
10 70 22 25 23 17 21 21 25 10
Test
Test Results
Filter 0 4396
Filter 1 4576
Filter 2 4522
Filter 3 4509
Filter 4 4407
Filter 5 4507
Filter 6 4520
Filter 7 4492
Filter 8 4465
Filter 9 4481
Accept
Cancel
02/10/2003
15:01

4.3.7.3. Repeatability without moving the filter wheel

To perform this and the following tests, the base line and darkness count test must have first of all been performed. This test takes absorbance readings during 1 minute with the filter wheel in fixed position. The technician can choose the rotor well on which he wishes to take the readings and fill it with the liquid he desires. He can choose which wavelength he wishes to use. The test can also be performed with the filter covered. When the readings end, the screen graphically displays the count numbers obtained and the absorbances with regard to the corresponding base lines. The program also shows the averages and/or standard deviations of the count numbers and the absorbances.

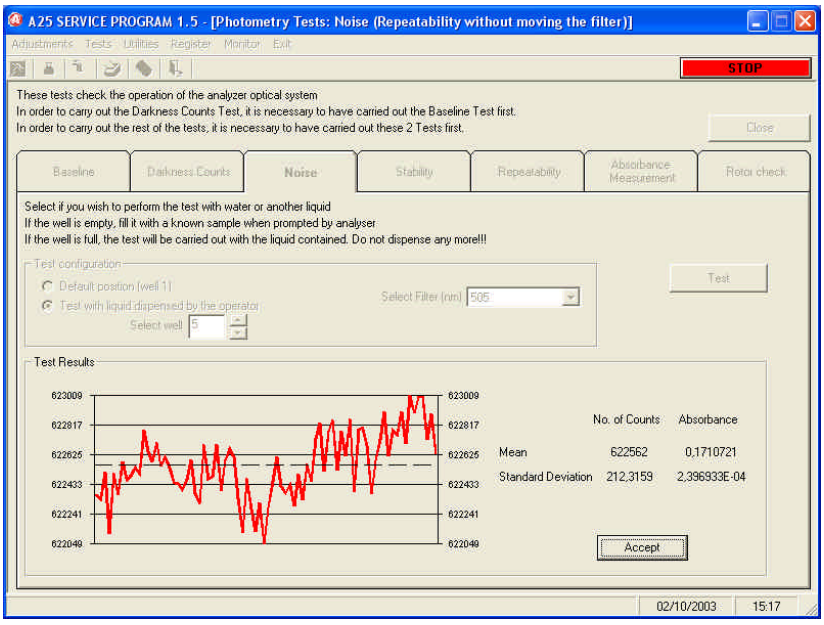
A25 SERVICE PROGRAM 1.5 - [Photometry Tests: Noise (Repeatability without moving the filter)]
Adjustments Tests Utilities Register Monitor Exit
STOP
These tests check the operation of the analyzer optical system
In order to carry out the Darkness Counts Test, it is necessary to have carried out the Baseline Test first.
In order to carry out the rest of the tests, it is necessary to have carried out these 2 Tests first.
Close
Baseline
Darkness Counts
Noise
Stability
Repeatability
Absorbance Measurement
Rotor check
Select if you wish to perform the test with water or another liquid
If the well is empty, fill it with a known sample when prompted by analyser
If the well is full, the test will be carried out with the liquid contained. Do not dispense any more!!!
Test configuration
Default position (well 1)
Test with liquid dispensed by the operator
Select well
Select Filter (nm) 505
Test
Test Results
No. of Counts Absorbance
Mean 622562 0,1710721
Standard Deviation 212,3159 2,396933E-04
Accept
02/10/2003
15:17

4.3.7.4. Stability

This test takes absorbance readings during 30 minute with the filter wheel in fixed position. The technician can choose the rotor well on which he wishes to take the readings and fill it with the liquid he desires. He can choose which wavelength he wishes to use. The test can also be performed with the filter covered. The test can be cancelled at any time. When the readings end, the screen graphically displays the count numbers obtained and the absorbances with regard to the corresponding base lines. The program also shows the averages and/or standard deviations of the count numbers and the absorbances.

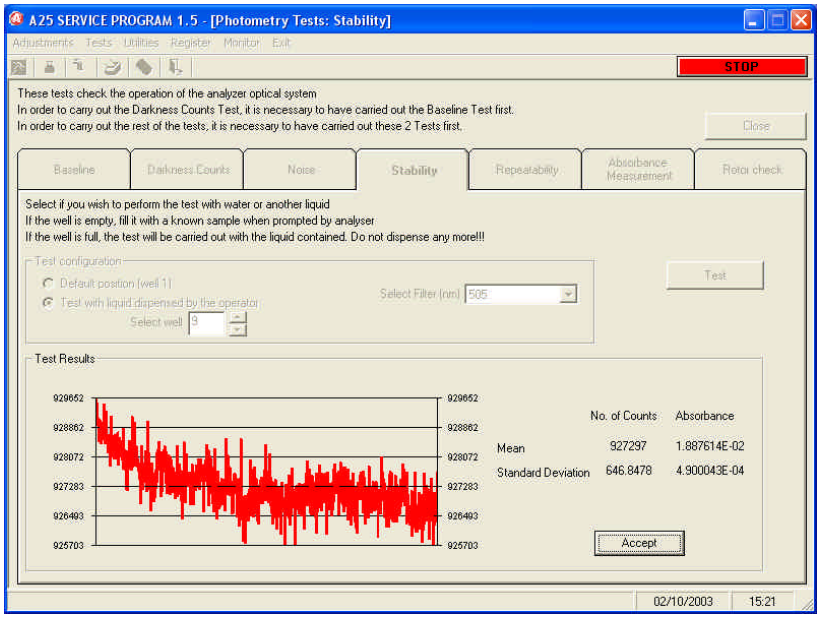
A25 SERVICE PROGRAM 1.5 - [Photometry Tests: Stability]
Adjustments Tests Utilities Register Monitor Exit
STOP
These tests check the operation of the analyzer optical system
In order to carry out the Darkness Counts Test, it is necessary to have carried out the Baseline Test first.
In order to carry out the rest of the tests, it is necessary to have carried out these 2 Tests first.
Close
Baseline
Darkness Counts
Noise
Stability
Repeatability
Absorbance Measurement
Rotor check
Select if you wish to perform the test with water or another liquid
If the well is empty, fill it with a known sample when prompted by analyser
If the well is full, the test will be carried out with the liquid contained. Do not dispense any more!!!
Test configuration
Default position (well 1)
Test with liquid dispensed by the operator
Select well
Select Filter (nm)
505
Test
Test Results
929652
928862
928072
927283
926493
925703
No. of Counts
Absorbance
Mean
927297
1.887614E-02
Standard Deviation
646.8478
4.900043E-04
Accept
02/10/2003
15:21

4.3.7.5. Repeatability moving filter wheel

This test takes absorbance readings during 10 minute moving the filter wheel randomly. The technician can choose the rotor well on which he wishes to take the readings and fill it with the liquid he desires. The test can be cancelled at any time. When the readings end, the screen graphically displays the count numbers obtained and the absorbances for each filter with regard to the corresponding base lines. The program also shows the averages and/or standard deviations of the count numbers and the absorbances for each filter.

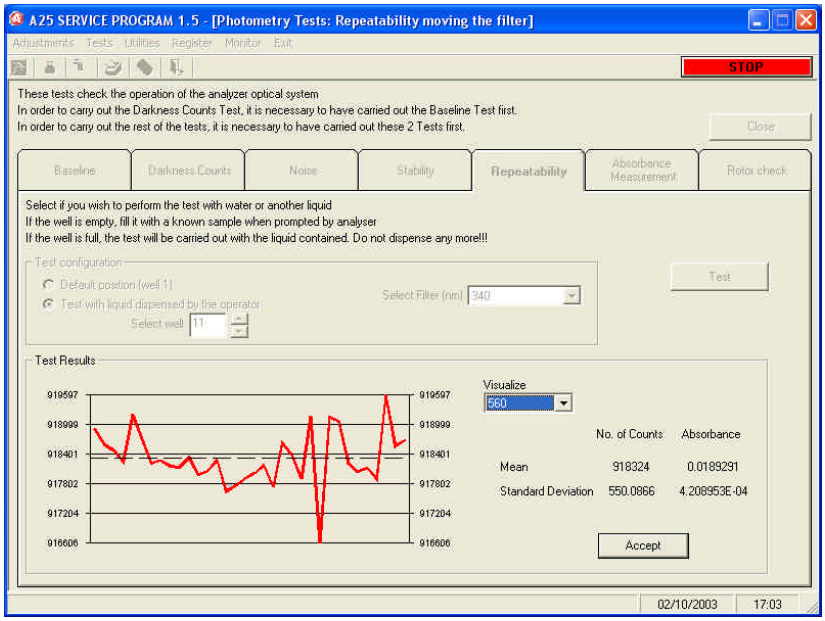

4.3.7.6. Absorbance measurement

This test enables individual absorbance readings. The technician can choose the rotor well on which he wishes to take the readings and fill it with the liquid he desires. He can choose which wavelength he wishes to use. The screen shows the count number obtained, the absorbance with regard to the corresponding base line, the value of the base line.

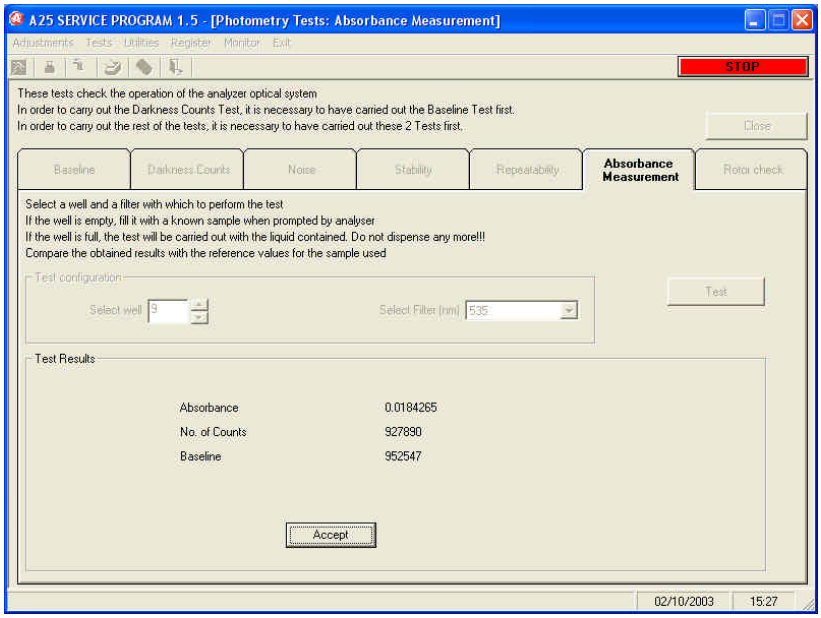
A25 SERVICE PROGRAM 1.5 - [Photometry Tests: Absorbance Measurement]
Adjustments Tests Utilities Register Monitor Exit
STOP
These tests check the operation of the analyzer optical system
In order to carry out the Darkness Counts Test, it is necessary to have carried out the Baseline Test first.
In order to carry out the rest of the tests, it is necessary to have carried out these 2 Tests first.
Close
Baseline
Darkness Counts
Noise
Stability
Repeatability
Absorbance Measurement
Rotor check
Select a well and a filter with which to perform the test
If the well is empty, fill it with a known sample when prompted by analyser
If the well is full, the test will be carried out with the liquid contained. Do not dispense any more!!!
Compare the obtained results with the reference values for the sample used
Test configuration
Select well
9
Select Filter (nm)
535
Test
Test Results
Absorbance
0.0184265
No. of Counts
927890
Baseline
952547
Accept
02/10/2003
15:27

4.3.7.7. Reactions rotor check

The user can use this test to check the optical status of a reactions rotor. He or she can choose the optical filter with which the test is to be performed. The technician must place the rotor in the analyzer and press the *Test* button. If the *Automatic Fill* option has been chosen, the analyzer fills the 120 rotor wells with distilled water and then makes a base line on each well with the chosen filter. The analyzer graphically displays the absorbances related to the average of all the wells and tells the technician the state of the rotor (optimal, adequate or unusable). After the test, the user must remove the rotor of the analyzer, empty it and dry it completely before using it for analyses.

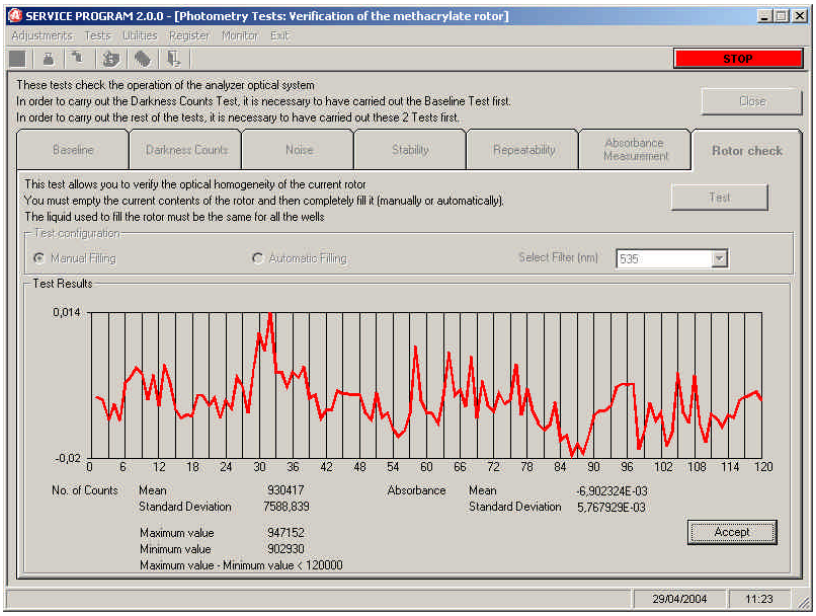
SERVICE PROGRAM 2.0.0 - [Photometry Tests: Verification of the methacrylate rotor]
Adjustments Tests Utilities Register Monitor Exit
STOP
These tests check the operation of the analyzer optical system
In order to carry out the Darkness Counts Test, it is necessary to have carried out the Baseline Test first.
In order to carry out the rest of the tests, it is necessary to have carried out these 2 Tests first.
Close
Baseline
Darkness Counts
Noise
Stability
Repeatability
Absorbance Measurement
Rotor check
This test allows you to verify the optical homogeneity of the current rotor
You must empty the current contents of the rotor and then completely fill it (manually or automatically).
The liquid used to fill the rotor must be the same for all the wells
Test
Test configuration
Manual Filling
Automatic Filling
Select Filter (nm)
535
Test Results
0,014
-0,02
0 6 12 18 24 30 36 42 48 54 60 66 72 78 84 90 96 102 108 114 120
No. of Counts
Mean 930417
Standard Deviation 7588,839
Maximum value 947152
Minimum value 902930
Maximum value - Minimum value < 120000
Absorbance
Mean -6,902324E-03
Standard Deviation 5,767929E-03
Accept
29/04/2004
11:23

4.3.8. Level control scales test

This screen makes it possible to check the functioning of the level control scales of the waste and distilled water containers. The technician must select which scales he wishes to check and place a certain amount of liquid in the corresponding container. On pressing the *Test* button, the screen shows the level of liquid measured by the analyzer(only 0 % and 100%)

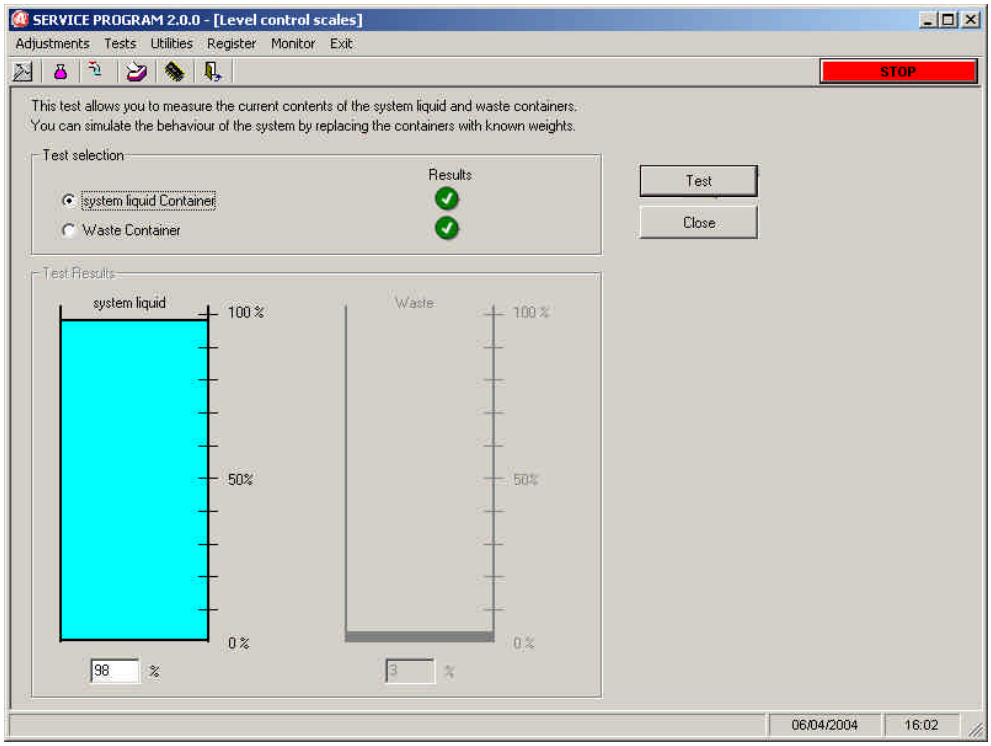

4.3.9. Covers detection test

This test makes it possible to check the functioning of the different detectors incorporated in the analyzer.

- Open detector of the general cover of the analyzer.
  Rotor cover presence detector.

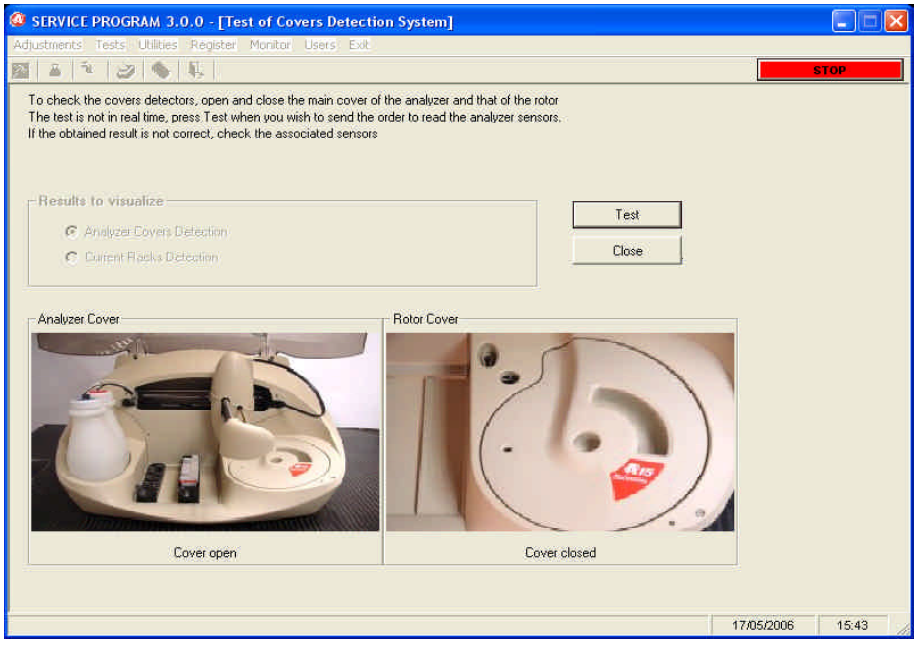
SERVICE PROGRAM 3.0.0 - [Test of Covers Detection System]
Adjustments Tests Utilities Register Monitor Users Exit
STOP
To check the covers detectors, open and close the main cover of the analyzer and that of the rotor
The test is not in real time, press Test when you wish to send the order to read the analyzer sensors.
If the obtained result is not correct, check the associated sensors
Results to visualize
Analyzer Covers Detection
Current Racks Detection
Test
Close
Analyzer Cover
Rotor Cover
Cover open
Cover closed
17/05/2006
15:43

The technician can manipulate the corresponding components, for example, open and close the cover of the analyzer and the screen shows the state of the detectors in each case.

4.3.10. PC-Analyzer communications channel test

On pressing the *Test* button, the computer attempts to establish communication with the analyzer. The program tells the technician if it has been possible or not.
The technician can select *Automatic Configuration* or *Manual Configuration*. In the case of the latter, he can define the *Port* and the *Speed*.

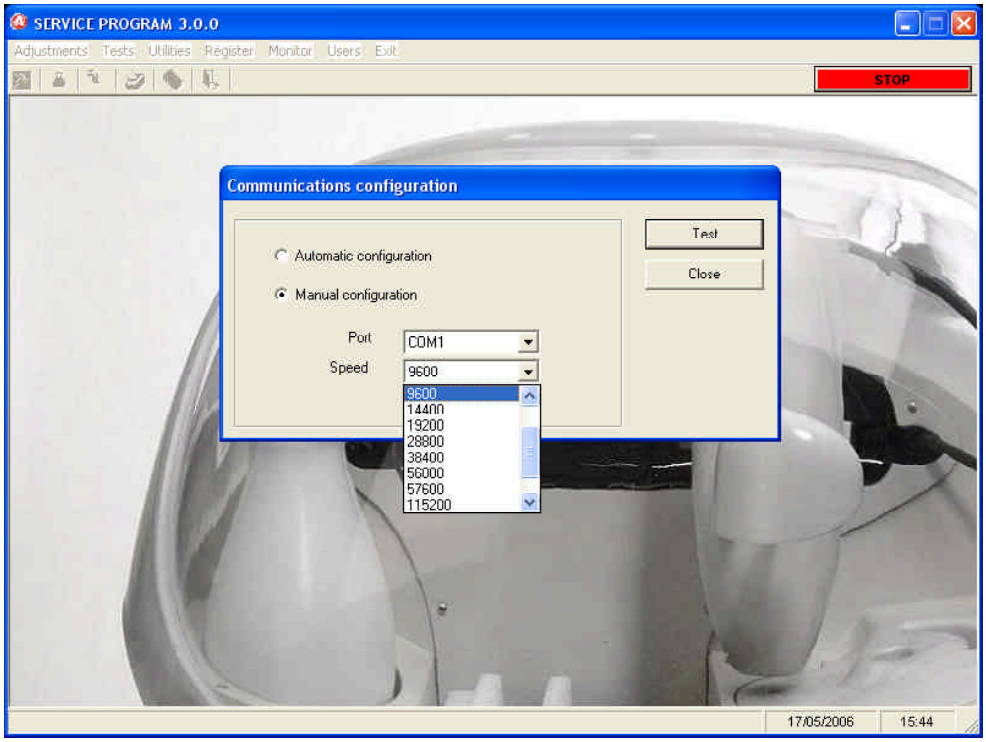

4.3.11. Global stress mode of the analyzer

This test makes it possible to continually reproduce work cycles of the analyzer similar to those made during the preparation and reading of reactions in a normal working routine, but dispensing at the washing station instead of the rotor. It is necessary for the dispensing system to be primed so that the piston does not function dry. All the racks must be removed from the racks tray. This test can be made without the covers and housing of the analyzer.
The technician can program the number of cycles he wishes (1 cycle = 15 seconds). The test can be cancelled at any time.
Once the test has been launched, the screen provides regular information about the current status of the process. If an error occurs during the process, the test ends and the screen displays a message indicating the element causing the error.
Partial stressing of the elements of the analyser is possible. The following elements can be stressed partially:

- X axis
- Y axis
- Z axis
- Reactions rotor
- Filter wheel
- Dispensation pump
- Membrane pumps
- 2-way electrvalve
- 3-way electriovalve

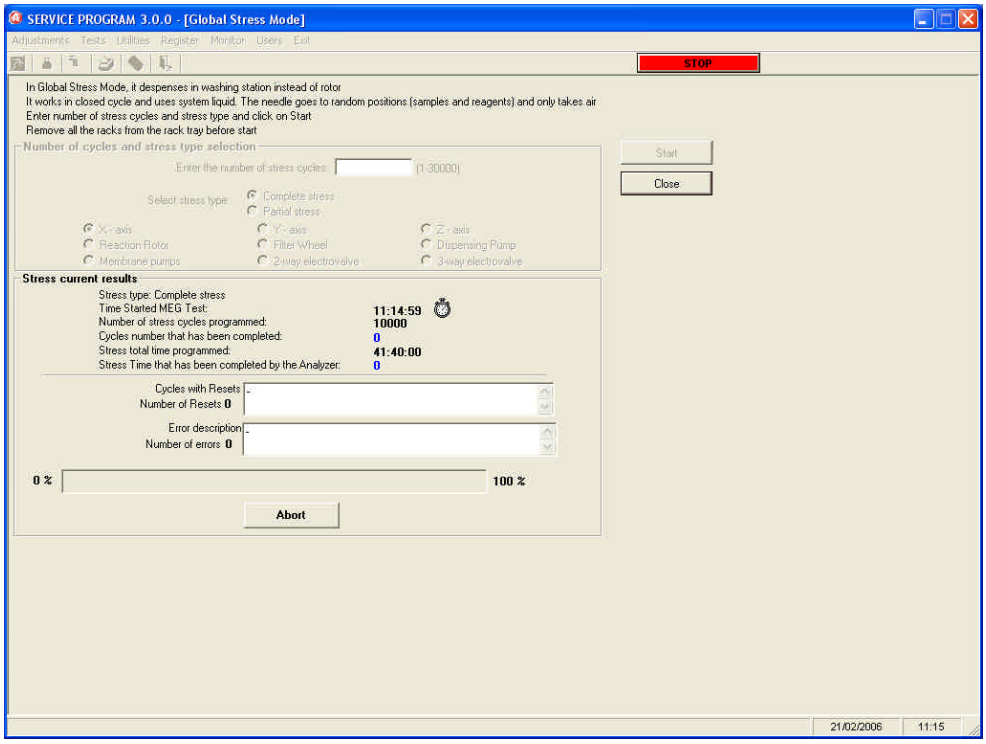

4.4. UTILITIES

The program contains various technical utilities. These utilities are also accessible from the user program.

4.4.1. Disassembly of the dispensing needle

On clicking on the Disassemble Needle button, the operating arm positions itself over the rack tray. The program

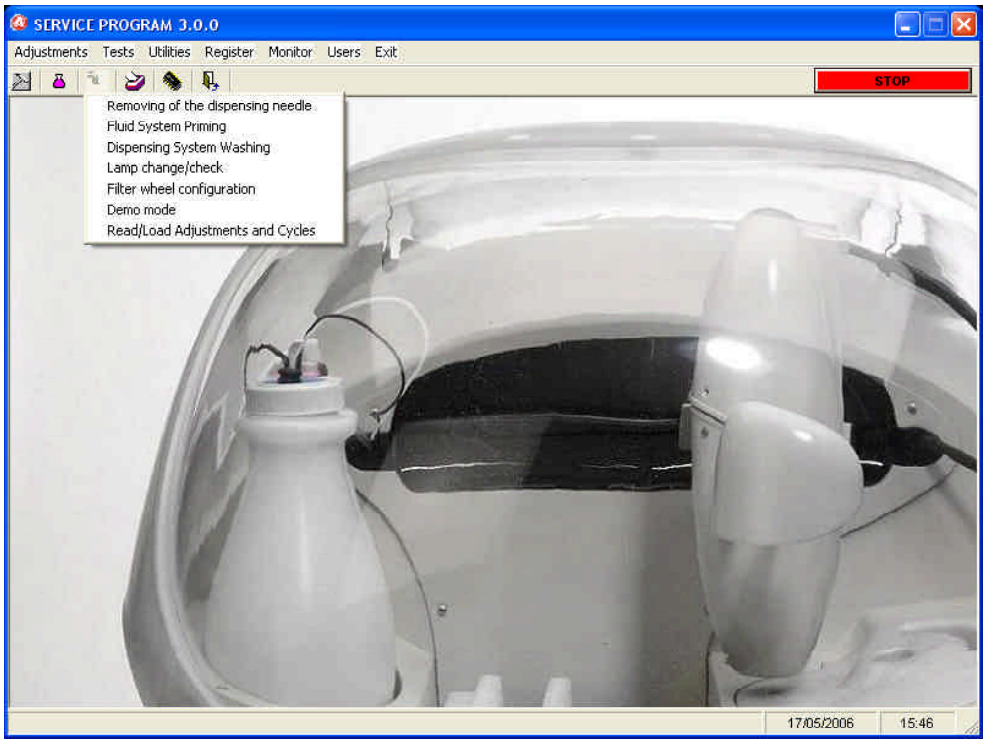

alerts the technician to remove any object positioned under the arm. On clicking OK, the needle descends and the technician can remove it to work with it or change it. To remove the needle, unscrew it by holding the top fitting. If, while handling the needle, the carriage rises due to the pressure made by the technician, press the Lower Needle button for the needle to descend once again. Once the needle has been reassembled on the analyzer, press the

Park button for the needle to rise. It performs the self-centering test and the arm finally returns to its parked position. These operations must be done with utmost care since they are carried out with the analyzer cover open and the needle may be contaminated. Laboratory gloves must always be used.

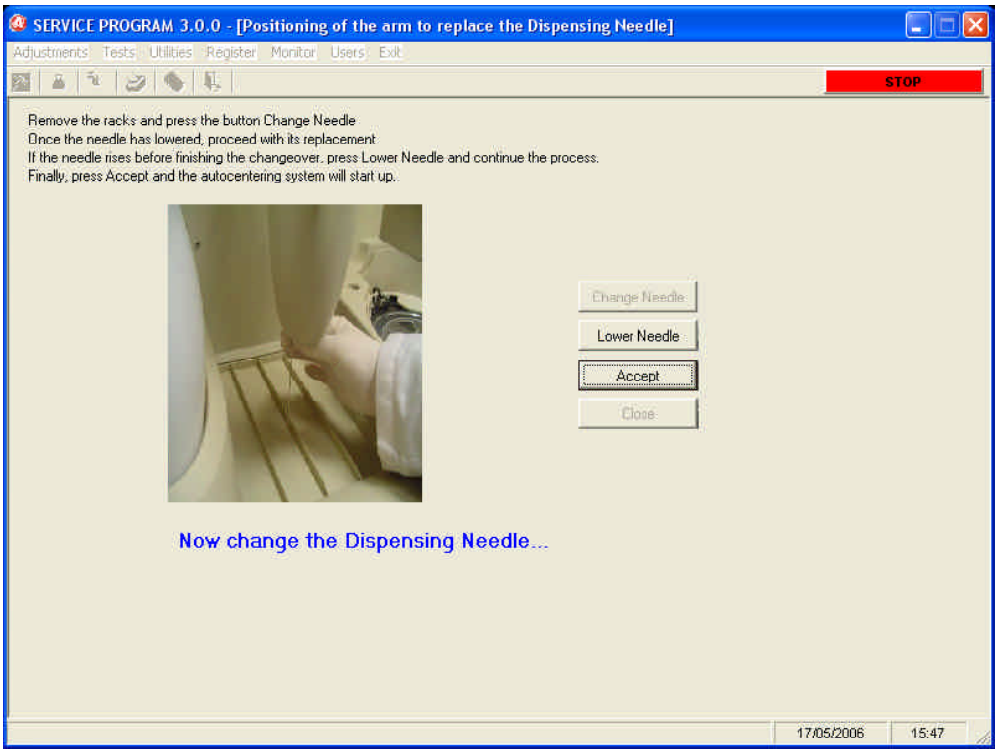
SERVICE PROGRAM 3.0.0 - [Positioning of the arm to replace the Dispensing Needle]
Adjustments Tests Utilities Register Monitor Users Exit
STOP
Remove the racks and press the button Change Needle
Once the needle has lowered, proceed with its replacement
If the needle rises before finishing the changeover, press Lower Needle and continue the process.
Finally, press Accept and the autocentering system will start up.
Change Needle
Lower Needle
Accept
Close
Now change the Dispensing Needle...
17/05/2006
15:47

4.3.2. Fluid system supply

On pressing the *Test* button, the analyzer fills the conduits of the dispensing system and the washing station with distilled water. To perform this operation, the operating arm is moved to the washing station. The technician can choose whether he wishes to prime the dispensing system, the washing system or both.

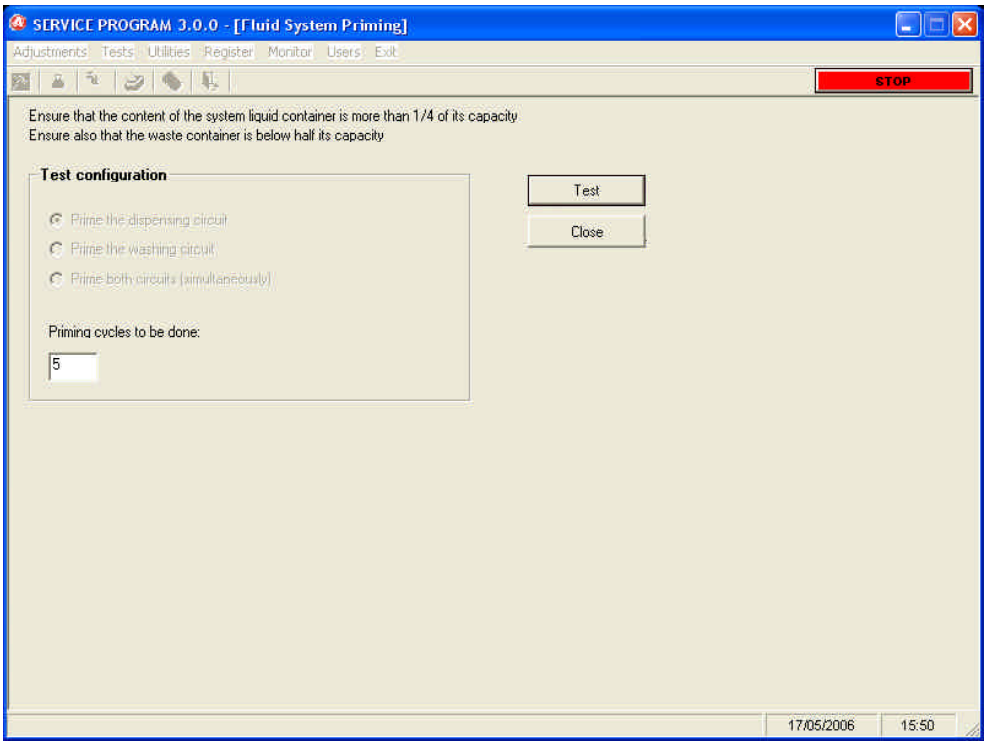
SERVICE PROGRAM 3.0.0 - [Fluid System Priming]
Adjustments Tests Utilities Register Monitor Users Exit
STOP
Ensure that the content of the system liquid container is more than 1/4 of its capacity
Ensure also that the waste container is below half its capacity
Test configuration
Prime the dispensing circuit
Prime the washing circuit
Prime both circuits (simultaneously)
Priming cycles to be done:
5
Test
Close
17/05/2006
15:50

4.3.3. Cleaning of the dispensing system

On pressing the *Wash* button, the analyzer washes the dispensing system internally and externally. To perform this operation, the operating arm is moved to the washing station. The technician can choose between performing the wash with distilled water or wash solution. In the case of the latter, the analyzer asks the technician to place a bottle of wash solution in stead of the distilled water container or to fill the latter with wash solution. Once the wash has been performed, the analyzer asks for the distilled water container to be put back in position. Finally, the analyzer primes the system with distilled water.

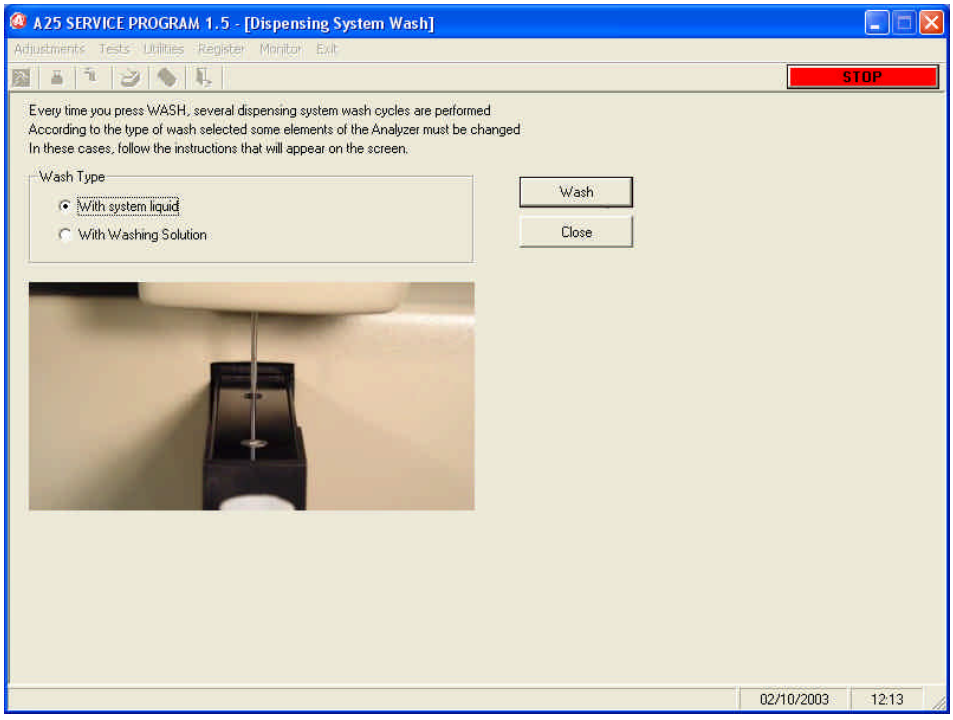
A25 SERVICE PROGRAM 1.5 - [Dispensing System Wash]
Adjustments Tests Utilities Register Monitor Exit
STOP
Every time you press WASH, several dispensing system wash cycles are performed
According to the type of wash selected some elements of the Analyzer must be changed
In these cases, follow the instructions that will appear on the screen.
Wash Type
With system liquid
With Washing Solution
Wash
Close
02/10/2003
12:13

4.3.4. Changing the lamp

When entering the screen, it is possible to choose between: Changing or checking the lamp. When a new lamp is

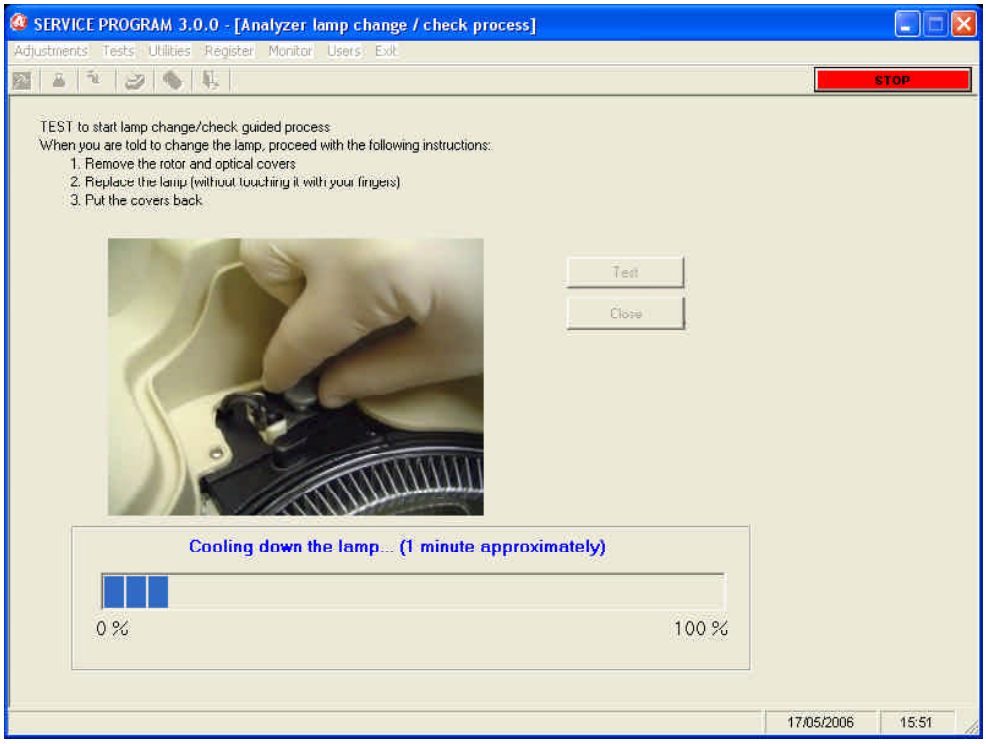
SERVICE PROGRAM 3.0.0 - [Analyzer lamp change / check process]
Adjustments Tests Utilities Register Monitor Users Exit
STOP
TEST to start lamp change/check guided process
When you are told to change the lamp, proceed with the following instructions:
1. Remove the rotor and optical covers
2. Replace the lamp (without touching it with your fingers)
3. Put the covers back
Test
Close
Cooling down the lamp... (1 minute approximately)
0 %
100 %
17/05/2006
15:51

installed, this utility must be used to notify the analyzer that the lamp has been changed and optimize the luminosity of the photometric system. The lamp must be changed with the analyzer in sleeping mode. If the analyzer is on standby mode, the program shuts it down automatically. The lamp must never be touched with fingers. Once the new lamp has been installed and the covers of the optic and rotor put back, access the change lamp utility and press the *Test* button. The program starts up the analyzer, checks the light intensity of the optical system, shuts down the analyzer and then requests the technician to remove the lamp holder again and replace it again turning it 180º on the axis of the lamp. If the temperature of the lamp holder is high, wait until it cools down or use pincers to hold it. The program starts up the analyzer again, measures the light intensity of the optical system again, compares the light intensity in both possible positions and chooses the greatest luminosity. If it is

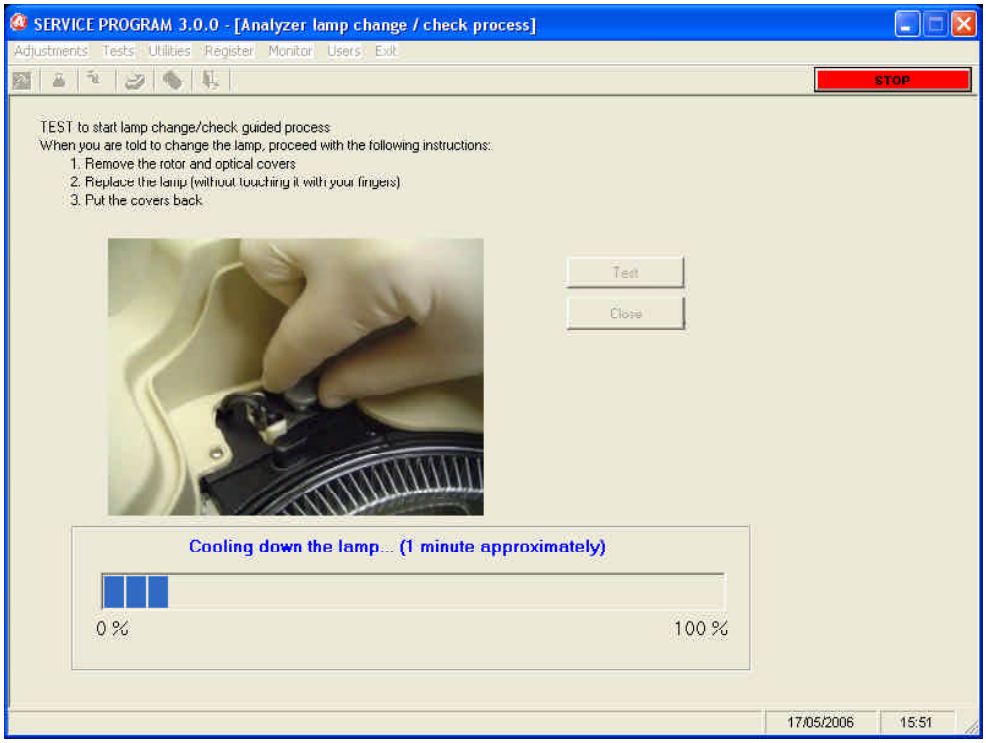

the current position, it tells the technician that the test is complete. If the best position were the previous one, the program shuts down the analyzer and asks the technician to remove the lamp holder and replace it, turning it 180º on the axis of the lamp, returning the lamp to its initial position. If the option selected at the beginning was to Check the Lamp, the process is the same but without shutting down the analyzer at the beginning.

4.3.5. Configuration of the filter wheel

This screen enables the modification of the analyzer filter wheel. The wheel has 10 positions. Position 0 must always contain a covered filter so that the analyzer can perform the darkness adjustment. Positions 1 to 9 can be used for optical filters. All the positions of the wheel must be occupied for it to work correctly. The positions that do not contain an optical filter must be occupied by a covered filter. The analyzer includes as standard 8 optical filters in positions 1 to 8 and two covered filters in positions 0 to 9. If one of the filters is to be changed, select the desired position of the wheel and press the Change Filter button. The analyzer automatically positions the filter wheel appropriately so that the technician can change the filter through the window of the optical system. Next, if it is

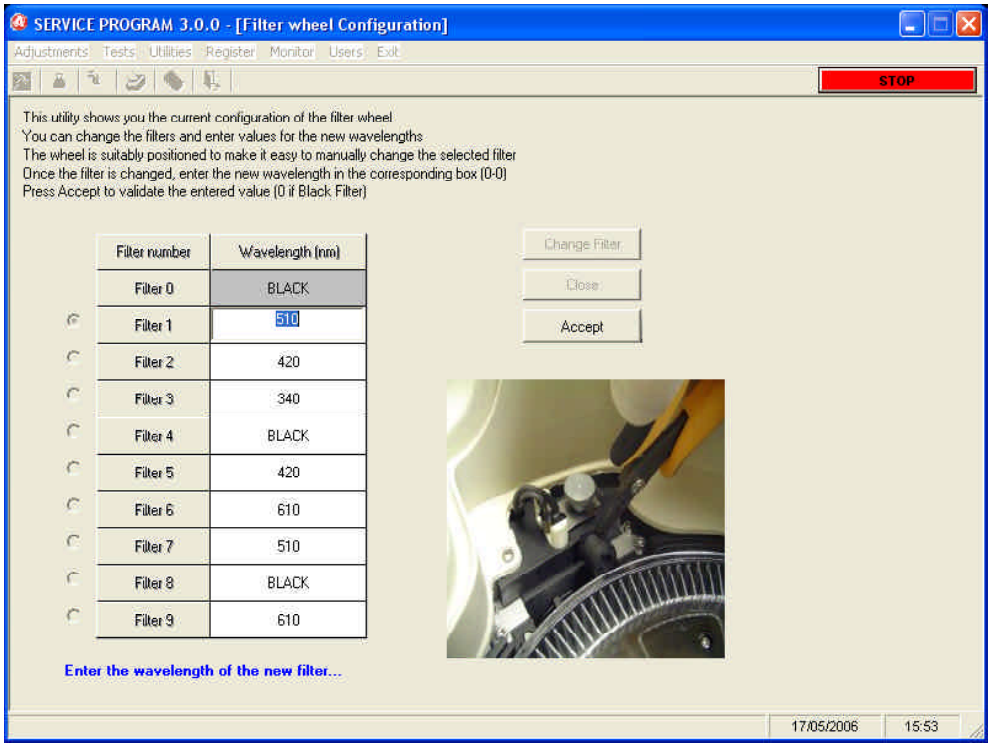
SERVICE PROGRAM 3.0.0 - [Filter wheel Configuration]
Adjustments Tests Utilities Register Monitor Users Exit
STOP
This utility shows you the current configuration of the filter wheel
You can change the filters and enter values for the new wavelengths
The wheel is suitably positioned to make it easy to manually change the selected filter
Once the filter is changed, enter the new wavelength in the corresponding box (0-0)
Press Accept to validate the entered value (0 if Black Filter)
Filter number
Wavelength (nm)
Filter 0 BLACK
Filter 1 510
Filter 2 420
Filter 3 340
Filter 4 BLACK
Filter 5 420
Filter 6 610
Filter 7 510
Filter 8 BLACK
Filter 9 610
Change Filter
Close
Accept
Enter the wavelength of the new filter...
17/05/2006
15:53

different, introduce the wavelength of the new filter that has been installed. If the filter is covered, introduce value 0. On closing the screen, the analyzer asks if the filters have actually been physically changed and a series of warnings are given to the technician telling him he must bear in mind whether or not he has changed a filter.

4.3.6. Demonstration mode

On pressing the *Start* button, the analyzer activates some of its mobile components, imitating functioning during a work routine. The activated mechanical components are the operating arm, the reactions rotor and the filter wheel. On pressing the *Cancel* button, the analyzer finishes the current cycle and returns to its rest position.

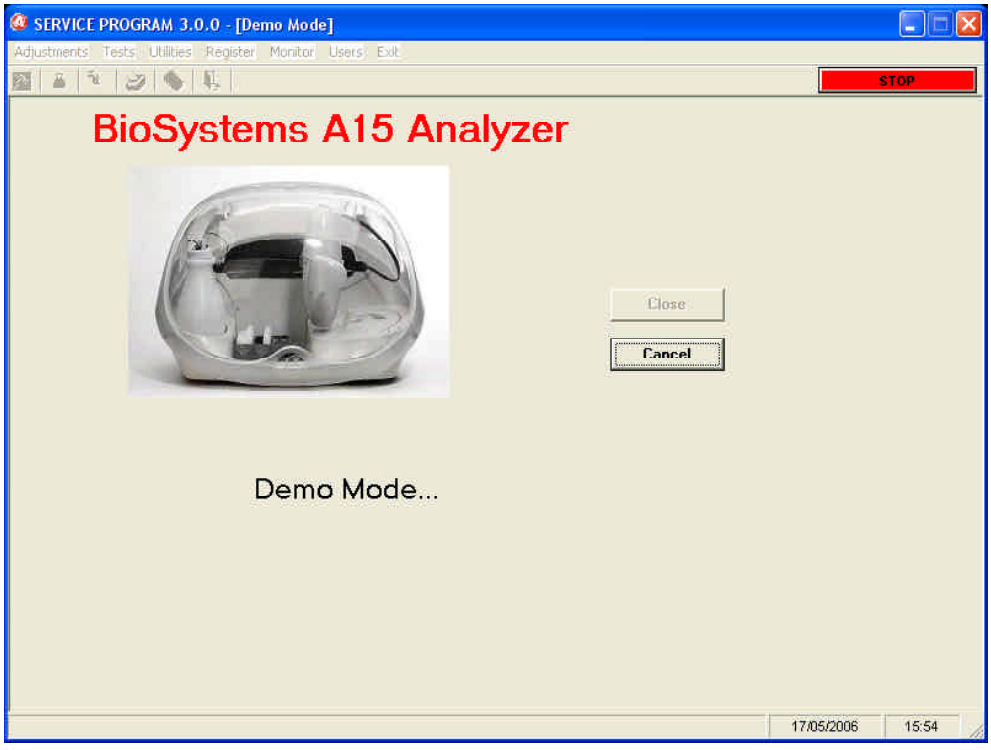

4.4.7 Read/load adjustments and cycles

From this screen, it is possible to read the current adjustments that the analyser is using by pressing the button Read Adjustments.

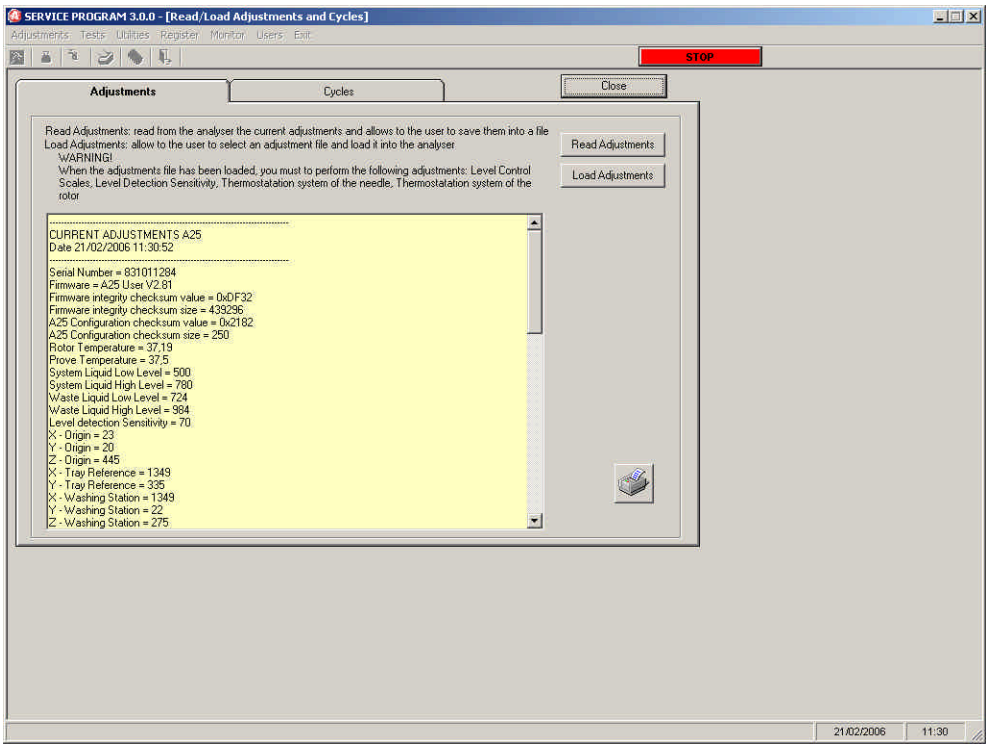
SERVICE PROGRAM 3.0.0 - [Read/Load Adjustments and Cycles]
Adjustments Tests Utilities Register Monitor Users Exit
STOP
Adjustments
Cycles
Close
Read Adjustments: read from the analyser the current adjustments and allows to the user to save them into a file
Load Adjustments: allow to the user to select an adjustment file and load it into the analyser
WARNING!
When the adjustments file has been loaded, you must to perform the following adjustments: Level Control Scales, Level Detection Sensitivity, Thermostatation system of the needle, Thermostatation system of the rotor
Read Adjustments
Load Adjustments
CURRENT ADJUSTMENTS A25
Date 21/02/2006 11:30:52
Serial Number = 831011284
Firmware = A25 User V2.81
Firmware integrity checksum value = 0xDF32
Firmware integrity checksum size = 439296
A25 Configuration checksum value = 0x2182
A25 Configuration checksum size = 250
Rotor Temperature = 37,19
Prove Temperature = 37,5
System Liquid Low Level = 500
System Liquid High Level = 780
Waste Liquid Low Level = 724
Waste Liquid High Level = 984
Level detection Sensitivity = 70
X - Origin = 23
Y - Origin = 20
Z - Origin = 445
X - Tray Reference = 1349
Y - Tray Reference = 335
X - Washing Station = 1349
Y - Washing Station = 22
Z - Washing Station = 275
21/02/2006
11:30

It is allowed to save these adjustments in a file. The technician selects the name and location of this file.
Also from this same screen and with the button Load Adjustments, the technician is allowed to select an adjustment file and to load it in the analyzer. Once the adjustment loading is made, the analyser turns off and the application is closed. When reinitiating the application, the new loaded adjustments will be already active.
From the firmware version 2.80, the programme counts the number of cycles of each element and the task of the analyser. From this menu, it is possible to read the cycles completed by the analyser. The screen displays the said cycles with the corresponding units.

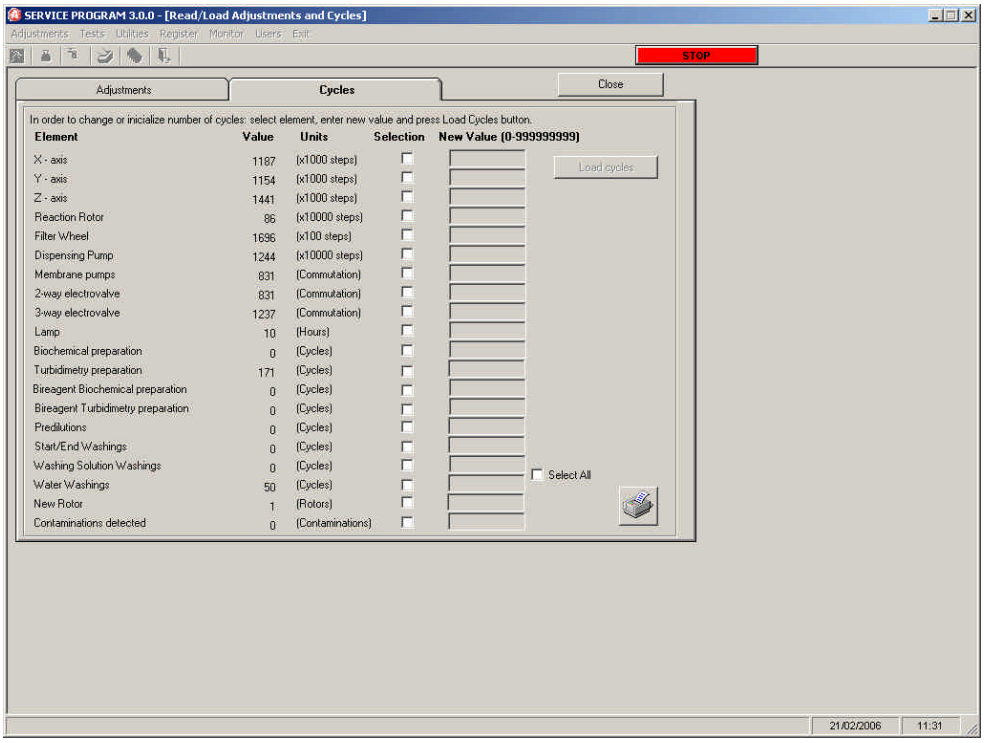
SERVICE PROGRAM 3.0.0 - [Read/Load Adjustments and Cycles]
Adjustments Tests Utilities Register Monitor Users Exit
STOP
Adjustments
Cycles
Close
In order to change or inicialize number of cycles: select element, enter new value and press Load Cycles button.
Element Value Units Selection New Value (0-999999999)
X - axis 1187 (x1000 steps)
Y - axis 1154 (x1000 steps)
Z - axis 1441 (x1000 steps)
Reaction Rotor 86 (x10000 steps)
Filter Wheel 1696 (x100 steps)
Dispensing Pump 1244 (x10000 steps)
Membrane pumps 831 (Commutation)
2-way electrovalve 831 (Commutation)
3-way electrovalve 1237 (Commutation)
Lamp 10 (Hours)
Biochemical preparation 0 (Cycles)
Turbidimetry preparation 171 (Cycles)
Bireagent Biochemical preparation 0 (Cycles)
Bireagent Turbidimetry preparation 0 (Cycles)
Predilutions 0 (Cycles)
Start/End Washings 0 (Cycles)
Washing Solution Washings 0 (Cycles)
Water Washings 50 (Cycles)
New Rotor 1 (Rotors)
Contaminations detected 0 (Contaminations)
Load cycles
Select All
21/02/2006
11:31

The programme automatically saves a copy of the adjustments and cycles read in a file. This file is located in the following folder:

c:\Program files\A15 Service\Adjustments\

When a physical element of the analyser has to be changed, e.g. the Z axis belt, the counter must be reset to zero for it to correspond to the number of cycles actually stored in the analyser. To perform this operation, select the box of the element that is to be initialised and enter the number of cycles in the enabled box. Then press the *Load cycles* button.
Using the *Load adjustments* button, this screen also enables the technician to select an adjustments file and load it in the analyser. When the adjustments are loaded, the cycles are also loaded. Perform this operation when a CPU board has to be changed. This avoids having to completely readjust the analyser; only the following sections will have to be readjusted:

- Scales
- Level detection sensitivity
- Needle thermostatation
- Rotor thermostatation

4.5. REGISTER

This enables the management of past adjustments, tests, incidences, repairs and maintenance of the instrument.

4.5.1. Introducing the analyzer serial number

The technician can enter the analyzer serial number so that it appears on printed service reports. If an entered serial number is changed, the service records are reinitiated. In this case, the technician can store all the previous data in a file.
The technician can enter his name so that it appears on the printed service reports.

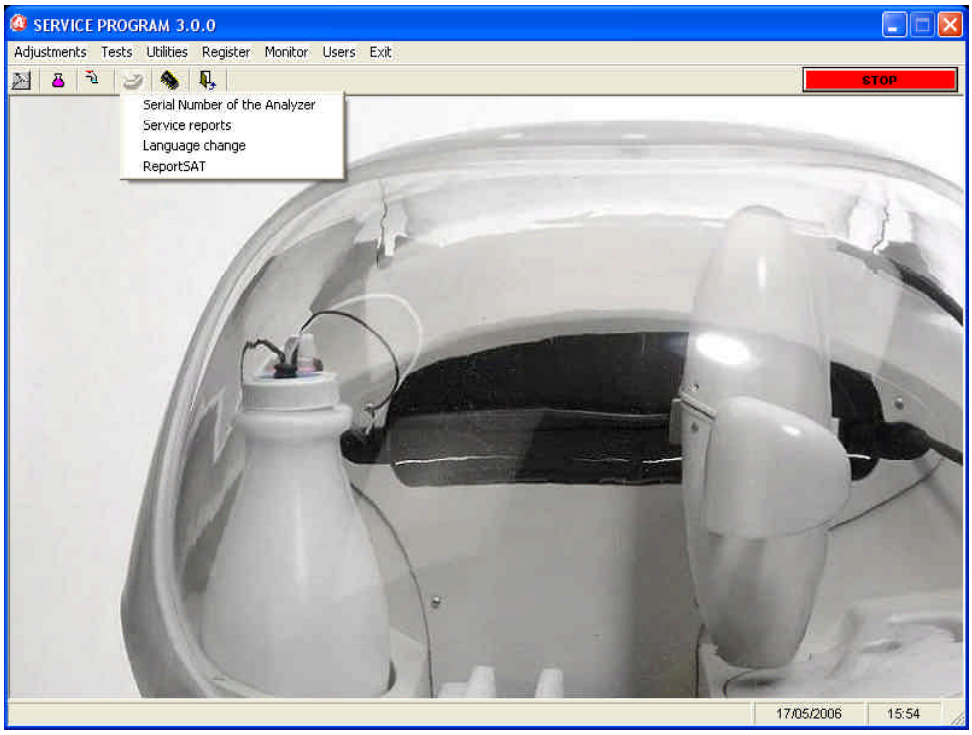

4.5.2. Service Reports

The program can display and print various service reports. The printed reports contain the analyzer serial number and the name of the current technician.

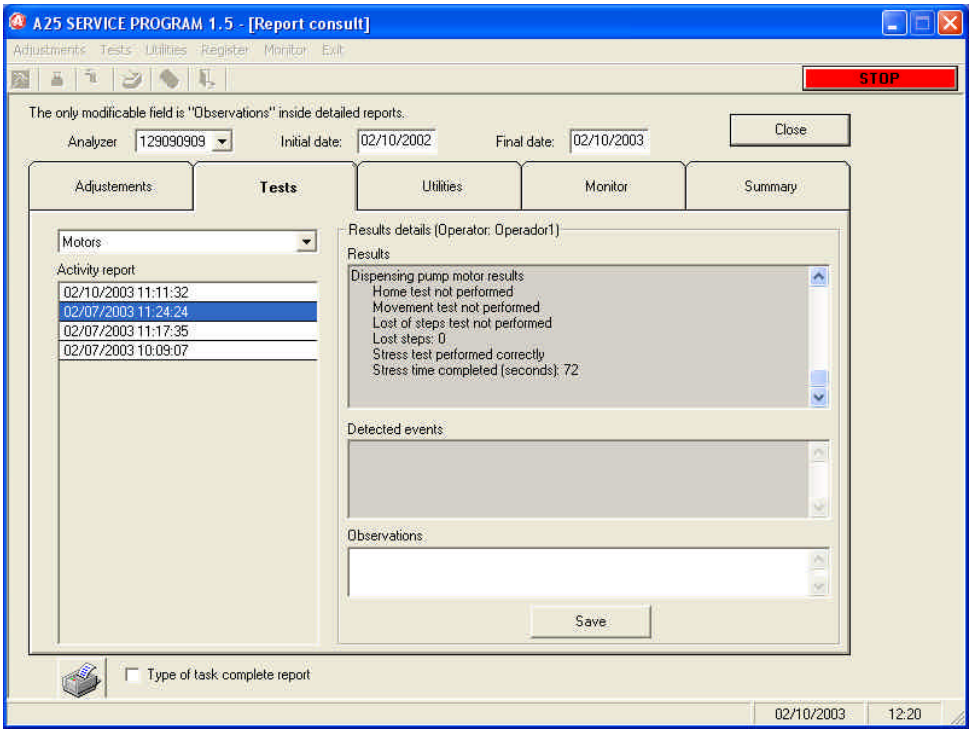

Reports are stored organised by: Adjustments, Tests, Utilities, Monitor and Summary of actions and tasks carried out.
In all cases, it is possible to select the actions carried out within a range of dates chosen by the technician.
The technician can enter short descriptions of the incidences that may happen in the analyzer and the repairs and maintenance operations that may be performed to the instrument in the Observations box.

4.5.3. Language change

This makes it possible to choose the language used in the service program.

4.5.4. Users

Two types of user can be created with different access levels:

· **SAT.** This user has full access to the programme. This user has permission to create and/or delete other users.
· **User.** This user has restricted access to the programme. This user can only perform the tests and run the utilities. He/she can not make any adjustments or load any previously saved adjustments files or change the firmware version of the analyser.

From the *Users* menu, it is possible to create, delete and change users. The *Change password* option is for each user to change his own password.

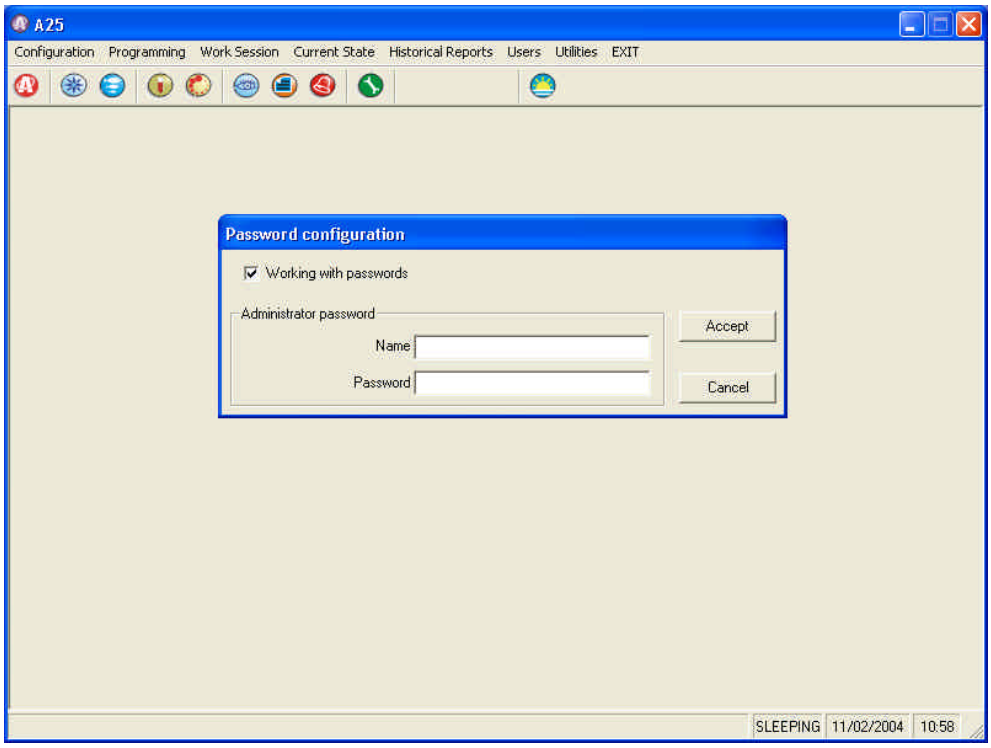

4.6. MONITOR

These enable the low level communication with the analyzer to load new versions of the program in the *flash* memory of the analyzer (*firmware*) or to restore the default adjustment parameters.
The firmware of the analyzer resides in a permanent flash memory. The change of this program can be made through the computer without the need for changing the memory chip. Once the program has changed, the analyzer is restarted with the new version of the program. While the copy process is being performed, the screen indicates the percentage completed. To load the new version, press the *Start* button, previously indicating where the program is located using the *Open* button. First of all, the current content of the flash memory is deleted and then the new program is loaded. This operation may take several minutes.
There is also the option to Restore Default Adjustments, selecting the option and pressing Start.
If the technician wants the analyzer to enter monitor mode (e.g. because the analyzer does not respond because the *firmware* was incorrectly loaded, he may do so by shutting down the analyzer, pressing the *Force Monitor* button and then rebooting.
Once the new programme has been loaded or the default adjustments have been restored, exit the monitor by pressing the *Close* button.

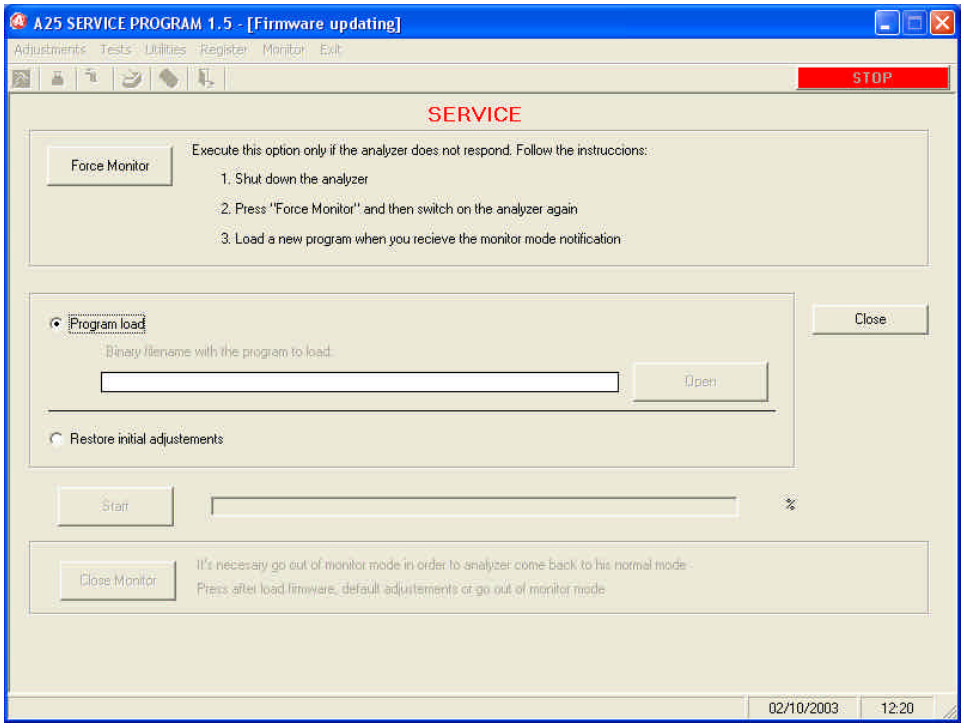
A25 SERVICE PROGRAM 1.5 - [Firmware updating]
Adjustments Tests Utilities Register Monitor Exit
STOP
SERVICE
Force Monitor
Execute this option only if the analyzer does not respond. Follow the instruccions:
1. Shut down the analyzer
2. Press "Force Monitor" and then switch on the analyzer again
3. Load a new program when you recieve the monitor mode notification
Program load
Binary filename with the program to load
Open
Close
Restore initial adjustements
Start
Close Monitor
It's necesary go out of monitor mode in order to analyzer come back to his normal mode
Press after load firmware, default adjustements or go out of monitor mode
02/10/2003
12:20

4.7 User's program

In this section, the service options in the user program will be described. These options are intended to configure the user's access level.
Each section explains how to manage and create different levels of access to the user program of the analyser.
When the program is installed for the first time, there is not a created user and access to the program is complete.

4.7.1 Configuration of the level of access to the analyser

To activate the option of level of access to the analyser, the first time you should enter as administrator, whose values are:

Name of user: **admin**
access key: **A15**

with this screen, the application with the operation by passwords is configured.
The first time that the program is activated, it forces the user to change the initial password.
It is possible to create three types of user with different access levels:

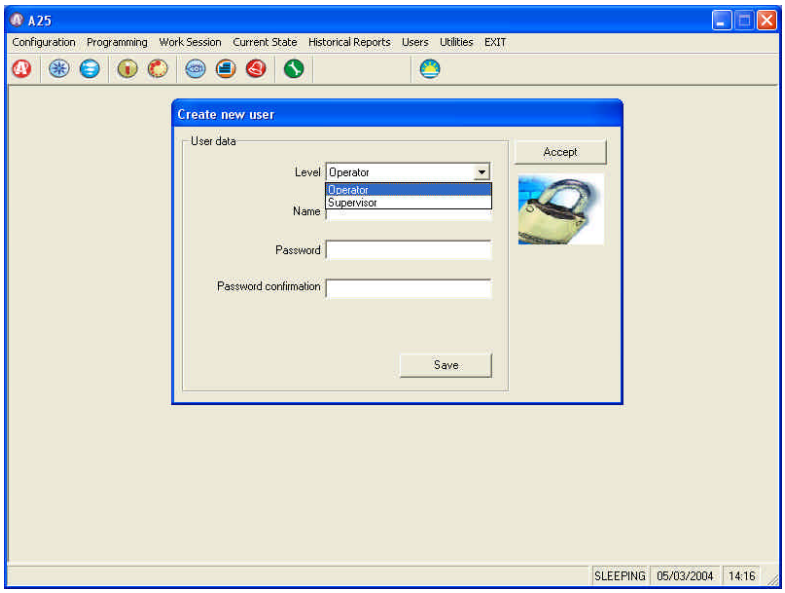

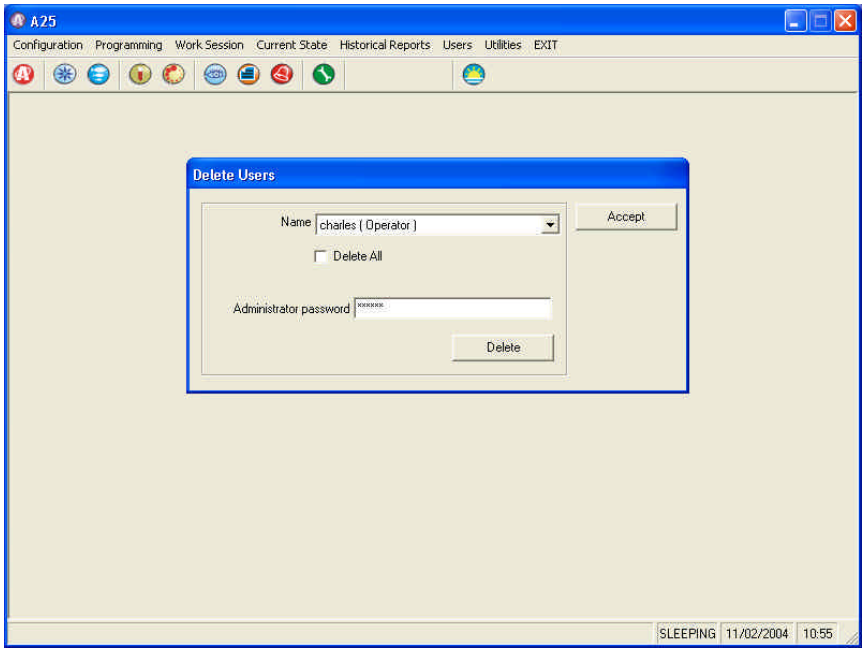

• **Operator**, is the user with a lower level of access to the application. He can only do working sessions, reports of current and historical results, and validate quality control results. In the screens of programming of techniques and contaminations, he can look up programming values, but he can not modify any parameter. He can not delete results or alarms. This user has total access to the rack and profile programming and to the analyser's configuration (except for changes of filters). He can change his own password.

• **Supervisor**, is the user with a medium access level. This user has got the same privileges as the operator user's and, in addition, he has got permissions to modify the programming of techniques in the calibration parameters and the control values. He can create a restricted number of new techniques, that is defined at the moment of creating such user and that it is a default setting of 5. He can also modify the programming of contaminations and change the analyser's filters. He can change his own password.

• **Administrator**, is the user with total access to the analyser's functions. He can create new users -as much at supervisor as at operator level-, eliminate or modify users. When creating supervisor users, he has to indicate the maximum number of new techniques that can create. He can activate or deactivate *Work Without Passwords* (option within the Configuration menu). He can also activate/deactivate the working without cover detection (this option is useful for the technical service to make verifications without needing to let the cover down). This option

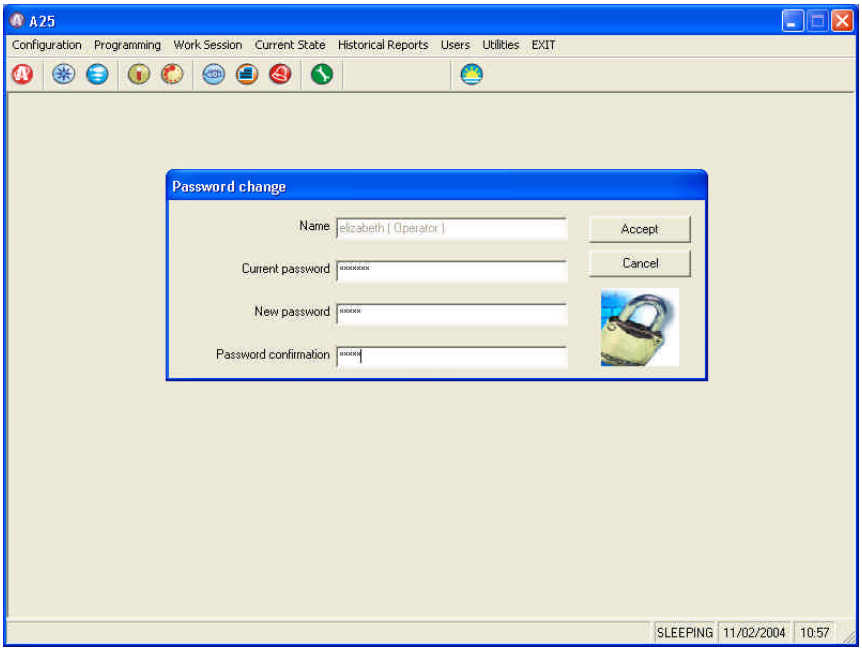

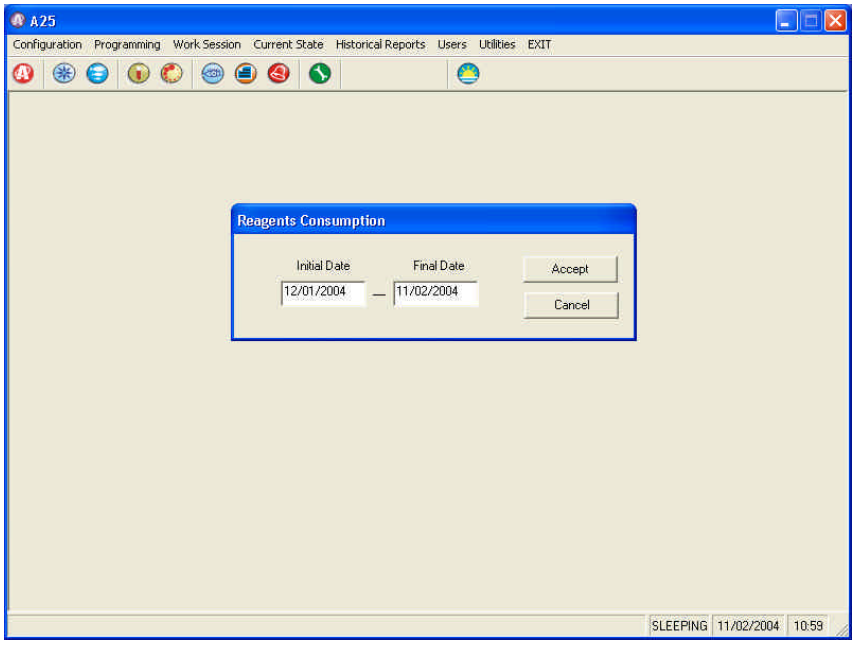

activates solely when the passwords are active.

When users are created, the access is limited to different parts of the program. When starting the program, an identification of the user is requested, by the user name and a password, and then the program will automatically restrict the different parts of the program depending on the access level permitted.
Whenever you want, you can change the user by means of the option *Change of user* from the User menu.
It is also allowed to eliminate users already created. Each user is capable of changing his password. All these options can be reached from the user menu.

4.7.2 Reagent Consumption

In order to access the consumption of reagents, it is first necessary to configure the program with the option of working with passwords. The administrator user is the only one that can access this menu -this option is deactivated for any other user.
In order to generate a list of the consumption of reagents, the administrator has to introduce the dates between which he wants to know the consumption. For this, it appears a screen like this:
Such option creates two files of results, one in text format *.txt* and the another one in excel format *.xls*. These files will be located at directory within the application directory, it will usually be:

c:\Program Files\A15\Reagents

and the contents of the file shows similar this:

REAGENT CONTROL CONSUME REPORT

Initial Date: 02/11/2004 Final Date: 02/12/2004

Test	Blank Prep.	Calibrator Pre	Control Prep.	Patient Prep.	Total Prep.	Vol. R1 (uL)	Vol. R2 (uL)
glucose	1	0	0	5	6	1332	0
alt	1	0	0	3	4	888	0
bilirrubin	9	0	0	23	32	7104	

3552*Reagents*

5. MAINTENANCE AND CLEANING

First of all, this chapter gives a step-by-step description of the different operations required for both the preventive maintenance and repair of the analyzer. The following are basic recommendations for the preventive maintenance of the instrument. Finally, a series of instructions for care and cleaning are given.

5.1. MAINTENANCE OPERATIONS

5.1.1. Housings and covers

5.1.1.1. Removing the needle unit casing

The needle unit has two casings fixed with four screws each
a) First remove the dispensing needle
b) Remove the screws that hold the casings in position.
c) Remove the upper casing by lifting upwards.
d) Remove the lower casing by pulling downwards.

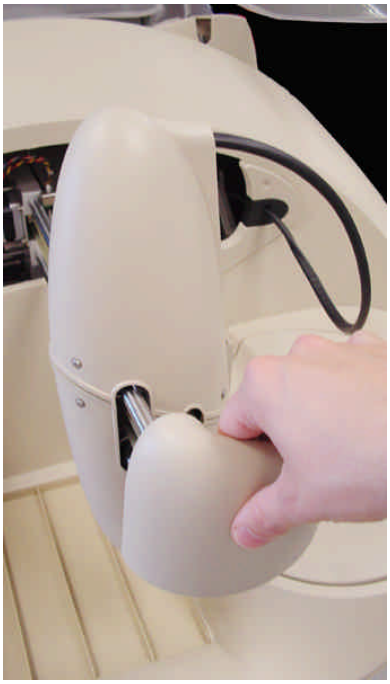

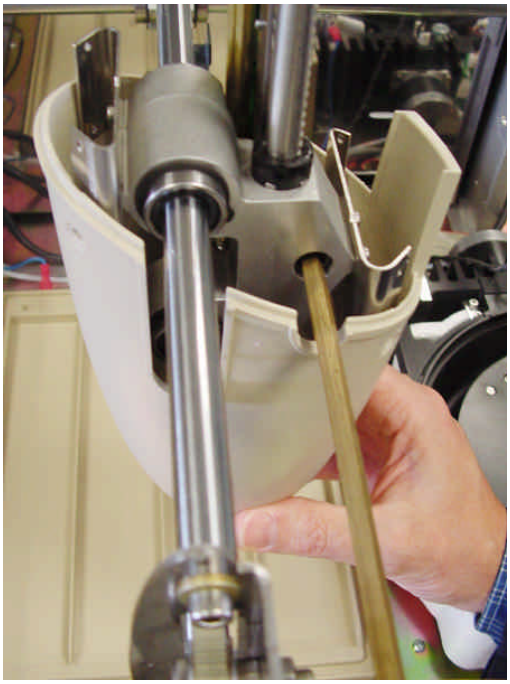

5.1.1.2. Removing the front housing

a) Remove the grommets on either side of the casing. Pull on the grommets, not on the hoses.
b) Remove the screws that hold the casing in position from the front.
c) Move the needle unit to its forward centre position.
d) Remove the casing by pulling it upwards and to the front.

5.1.1.3. Removing the main cover

a) Open the analyzer cover.
b) Remove the two bottom screws that hold the cover to each hinge.
c) Pull the cover upwards.

5.1.1.4. Removing the upper casing

a) Remove the front housing.
b) Remove the main cover.
c) Remove the screws as shown in the following figures.

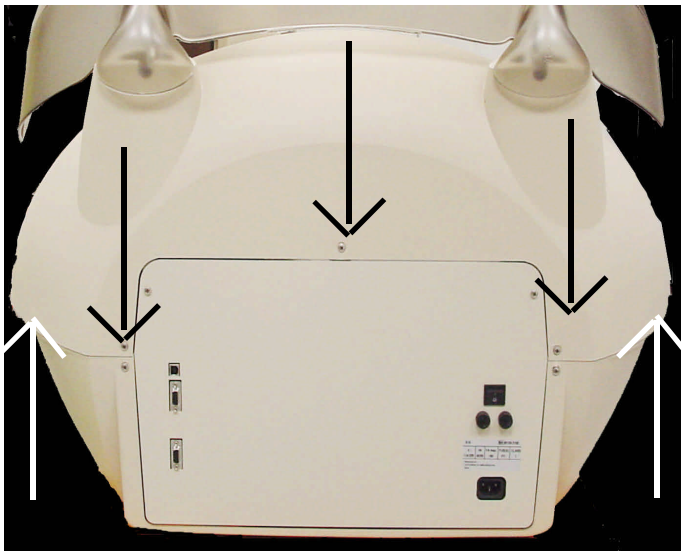

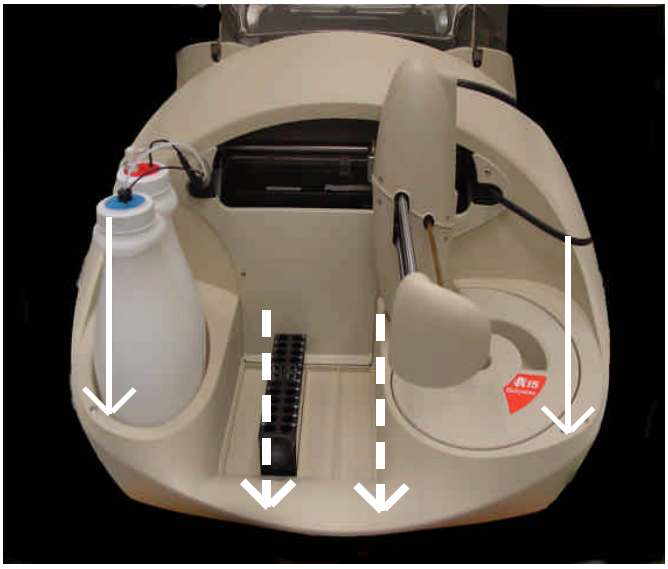

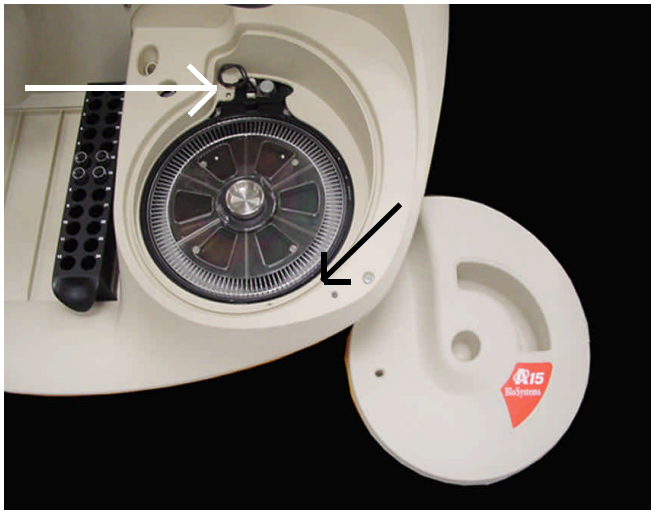

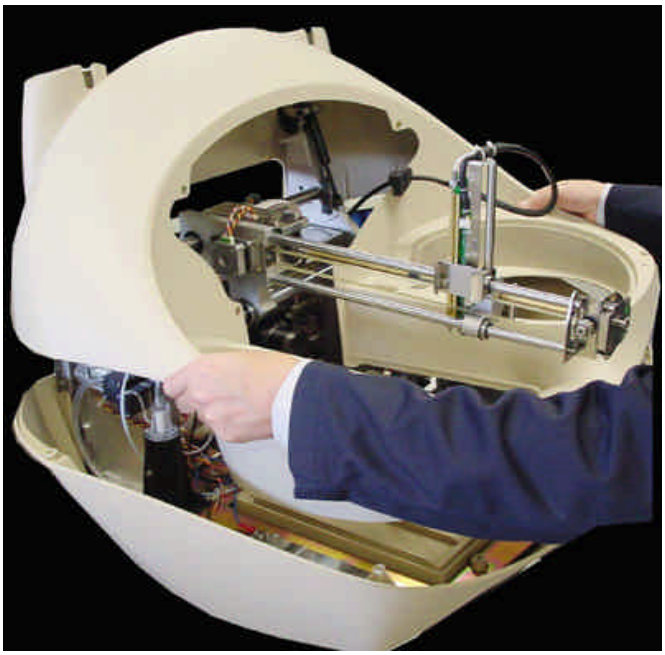

d) Remove the casing by pulling it upwards.

5.1.1.5. Removing the spring protector

a) Remove the three screws at the rear
b) Pull the protector upwards.

5.1.2. Operating arm

5.1.2.1. Fully removing the operating arm

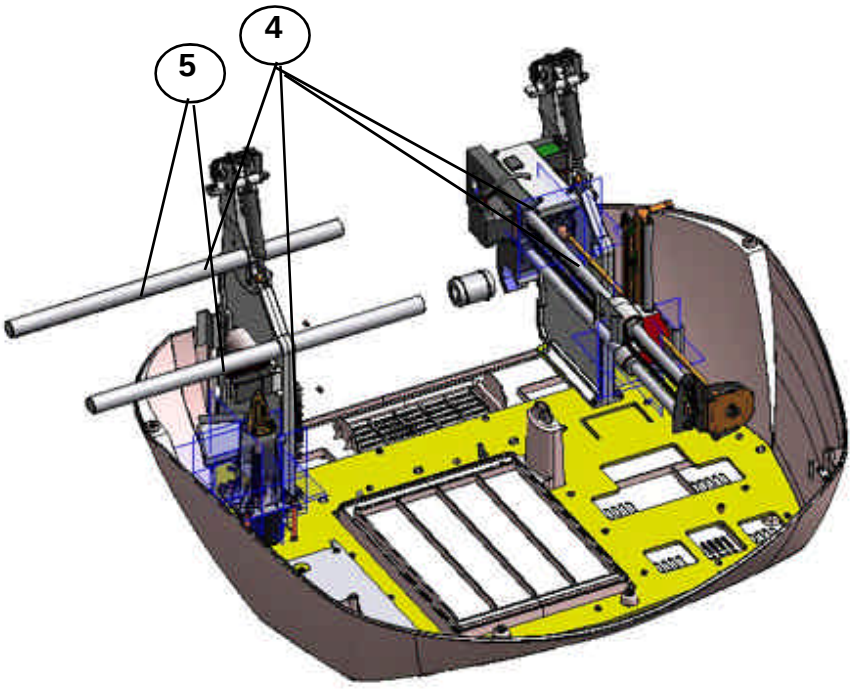

a) Remove all the analyzer housing.
b) Disconnect the connector (1) that goes to the board that goes to the needle unit and cut all the flanges required.
c) Disconnect the Teflon dispensing pipe (2).
d) Remove the cover that covers the X carriage interconnection board (3). Cut the flanges that hold the flat bands and disconnect them from the board.
e) Unscrew the four studs that fasten the two X guide axes and which are located on the arm supports.
f) Pull the two guide axes as shown in the figure.

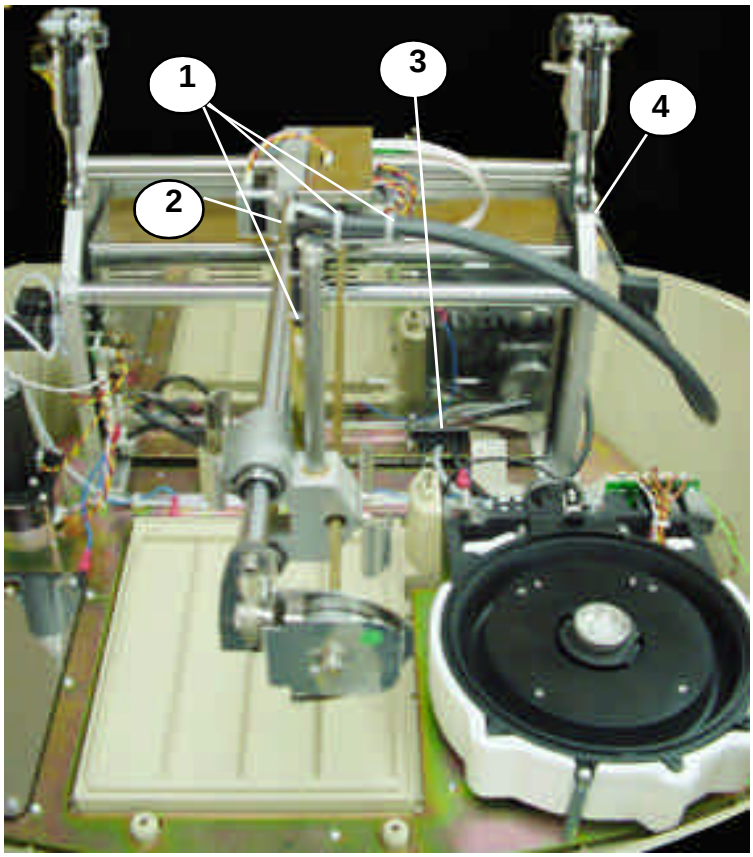

5.1.2.2. Changing the arm hose

a) Remove all the analyzer housing.
b) Disconnect the connector (1) that goes to the board that goes to the needle unit and cut all the flanges required.
c) Disconnect the Teflon pipe at both ends (needle and electrovalve) (2). Cut all the flanges that guide the pipe to the electrovalve.
d) Remove the cover (3). To do so, open the electronics box at the rear and remove the fastening clips. Disconnect the connector that goes to the CPU board and the earth connection (6).
e) Unscrew the flange screw (4).
f) Replace the hose, connect and replace the flanges.

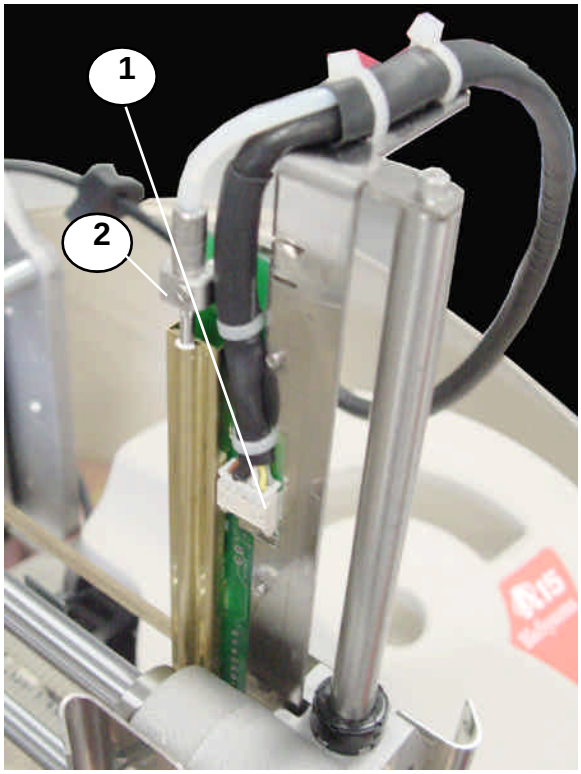

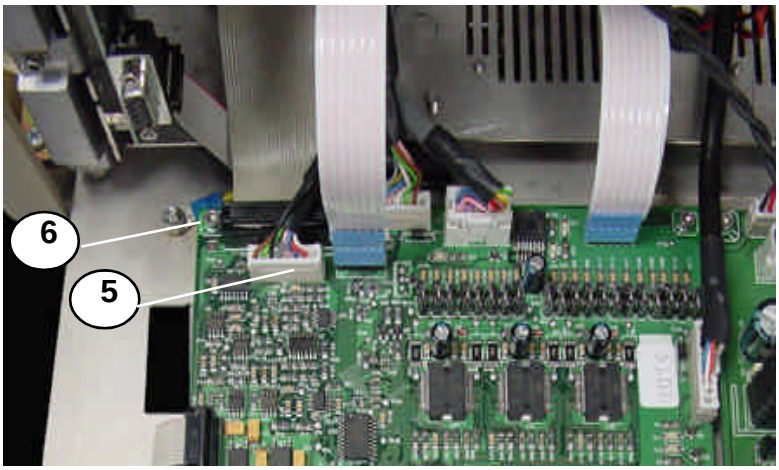

5.1.2.3. Changing the X motor

a) Remove all the analyzer housing.
b) Unscrew the studs (1).
c) Remove the rack (2) and let the arm rest on its front part.
d) Remove the cover and the interconnection board (3).
e) Remove the screws (4) and remove the motor.
f) Fit the new motor without fully tightening the screws.
g) Replace the rack.
h) Adjust the pinion (5) with the rack and tighten the screws.
i) Tighten the rack studs and fit the interconnection board and cover.

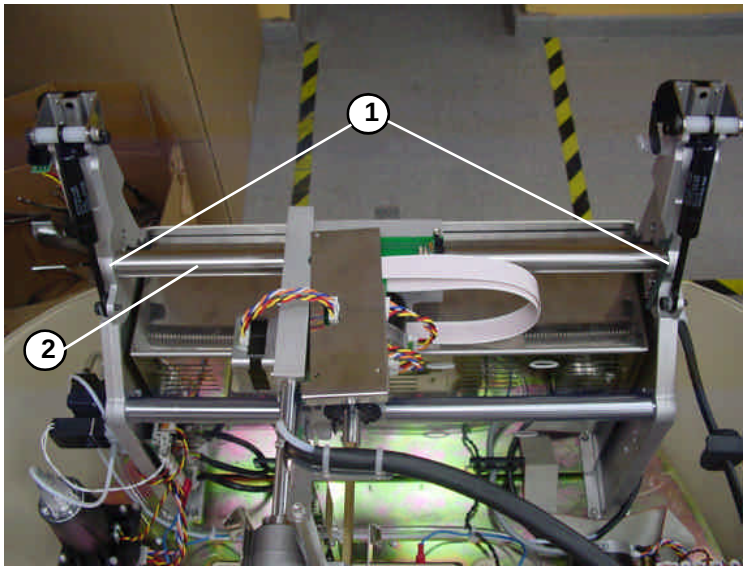
1
2

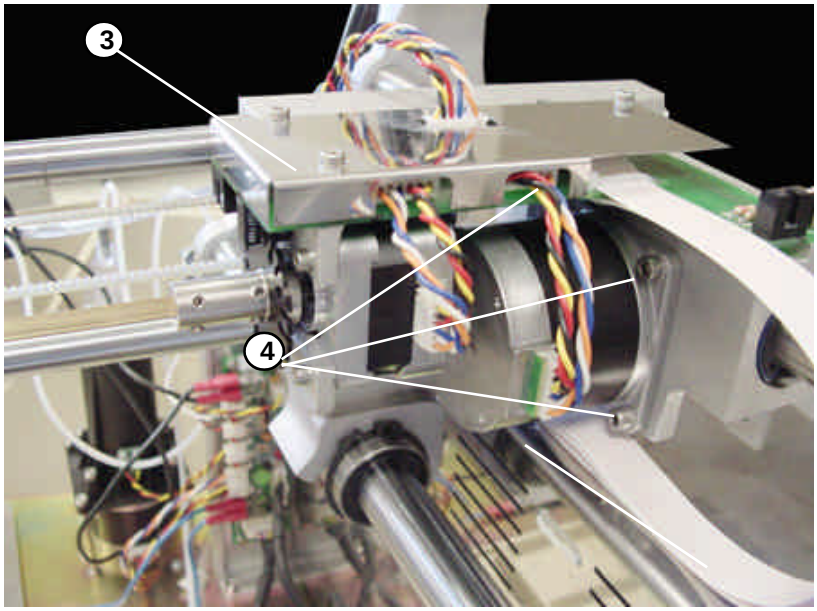
3
4

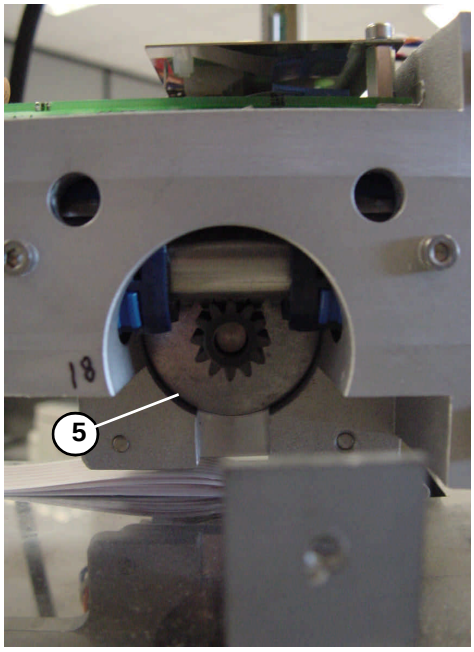
5

5.1.2.4. Changing the Y motor

a) Remove all the casings from the analyser except for that of the needle unit.
b) Connect the motor cable (1).
c) Remove the motor by removing the screws (2).
d) Change the motor (with pulley).
e) Remove the fastening plate (3).
f) Fit the fastening plate on the new motor.
g) Fit the motor without tightening the screws.
h) Connect the notched belt (4) , tighten it manually displacing the motor and tighten the 4 screws that hold it in position.
i) Connect the motor cable.

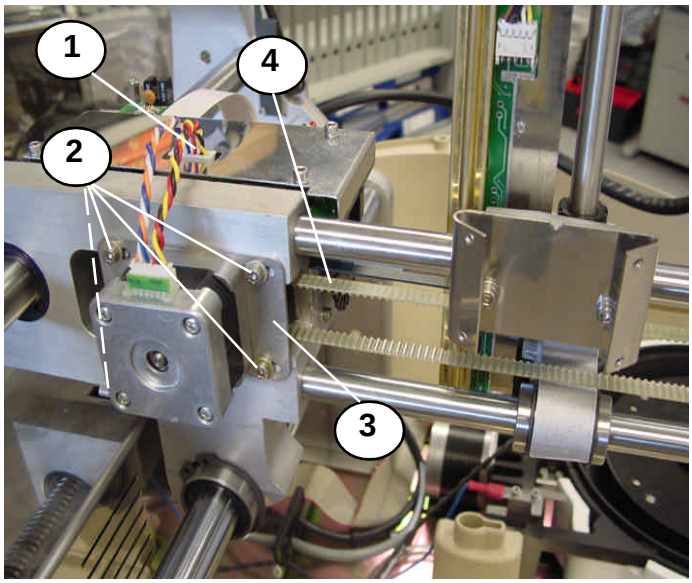

5.1.2.5. Changing the Z motor

a) Remove the X motor as explained in the section titled Changing the X motor.
b) Unscrew the two studs (1).
c) Remove the four screws that hold the motor in position (2).
c) Remove the connector and remove the motor by pulling it towards the rear.

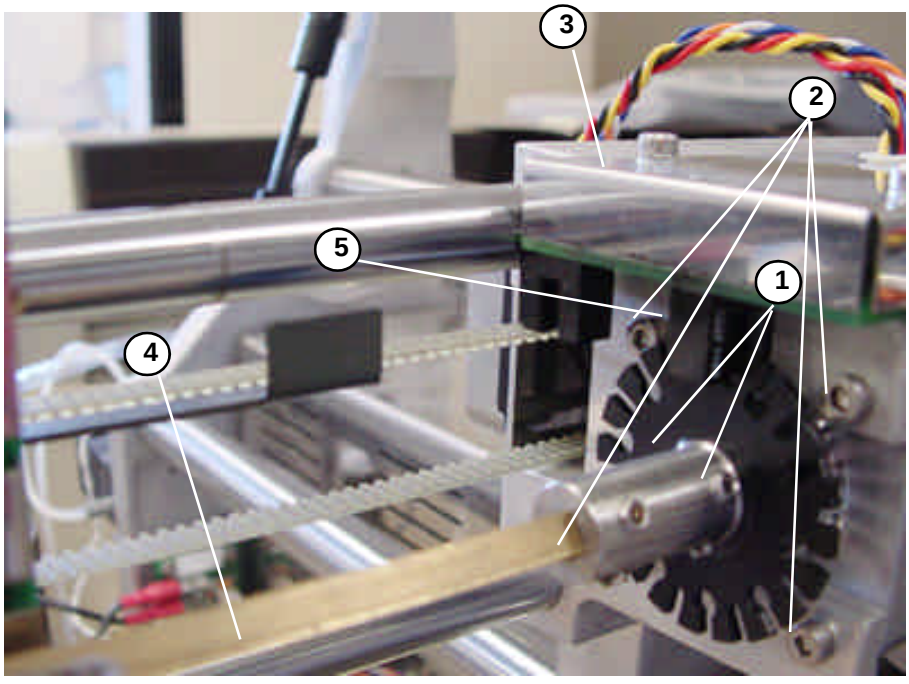

d) Remove the motor axle by unscrewing the stud.
e) Fit the axle to the new motor.
f) Refit the motor but without tightening the studs (1).
g) Fit the X motor and the interconnection board (3).
h) Adjust the axis (4) so that the encoder is centred on the photosensor (5) and tighten the studs (1).

5.1.2.6. Changing the Y motor belt

a) Loosen the Y motor (see section).
b) Remove the pulley (1) by extracting the bolt (2) and the nut (3).
c) Loosen the clamp that fastens the belt to the needle unit.
d) Change the belt for a new one.
e) Refit the pulley (1).
f) Put the belt on the pulleys, tighten it manually, displacing the motor and fasten it by tightening the 4 screws.

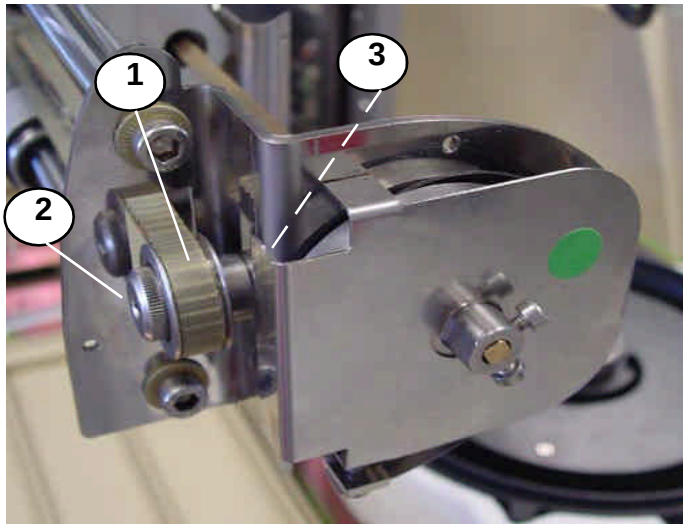

5.1.2.7. Changing the spring

a) Remove the pulley (1) as indicated in the section titled Changing the Y motor belt.
b) Unscrew the bolts (2).
c) Remove the bolts (3).
c) Remove the spring unit (4).
d) Refit the new unit but without tightening the studs (2). Make sure that the Y carriage axes are perfectly aligned.
e) Refit the pulley (1) as indicated in the section titled Changing the Y motor belt.

Tightening the spring:
f) During the following operations, keep the needle unit in its top position.
g) Use a spanner to turn the pulley (5) anticlockwise. Complete 3 to 4 turns.
h) Tighten the bolts (2) making them coincide with the flat part of the axle (6).

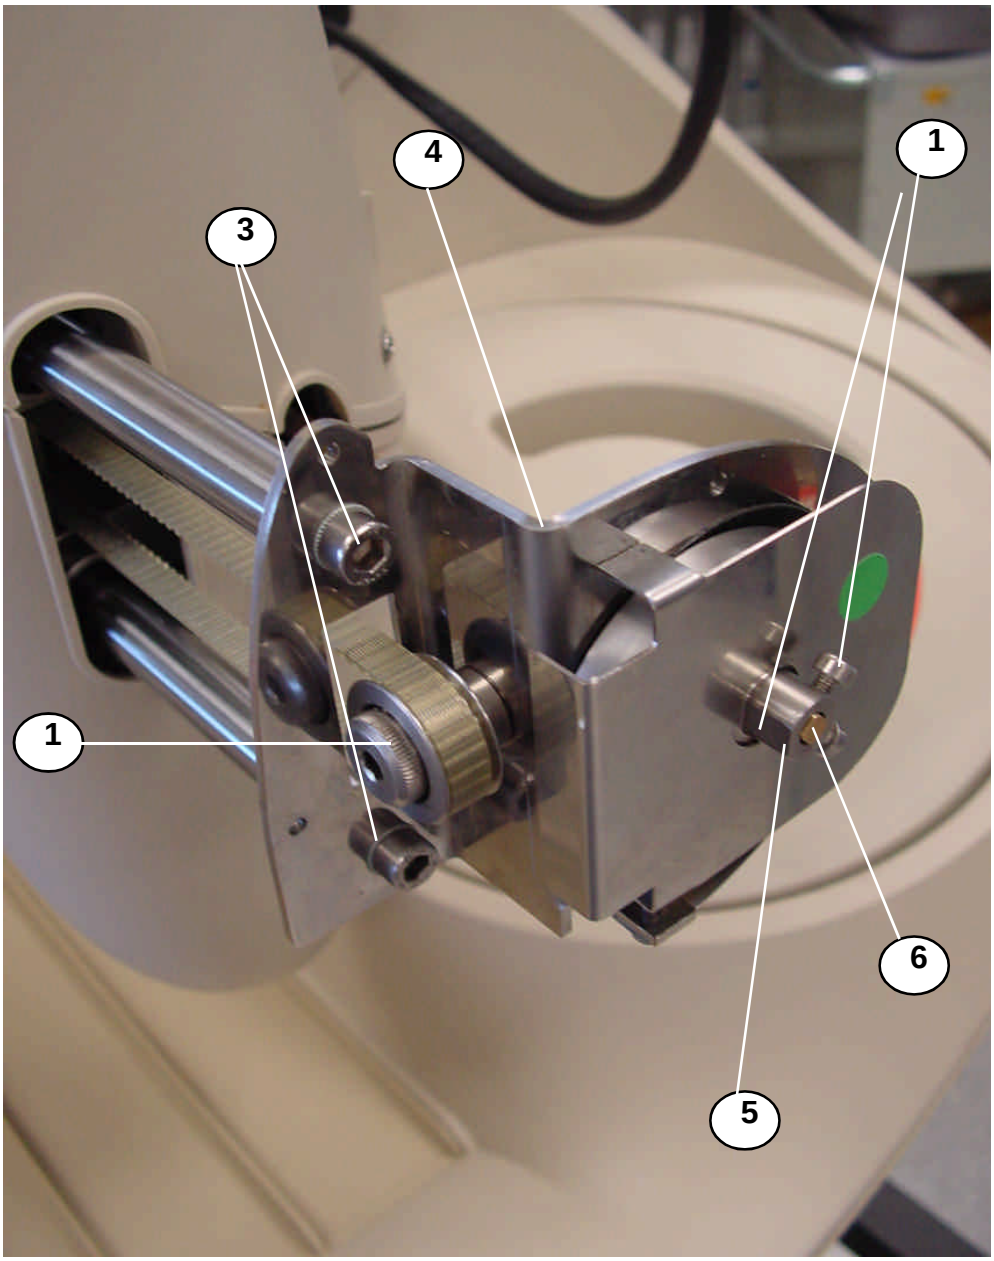

5.1.3. Dispensing system

5.1.3.1. Changing the thermostated pipe.

a) Remove the arm casing.
b) It is recommendable to remove the needle before handling the unit to prevent it from being damaged.
c) Disconnect the electrical connector (1) and the Teflon pipe (2) and remove the flanges (3).
d) Remove the protective cover (4).
e) Remove the entire thermostated pipe by removing the 3 screws (5) that hold it in place.
f) Refit the new unit, replacing the flanges.

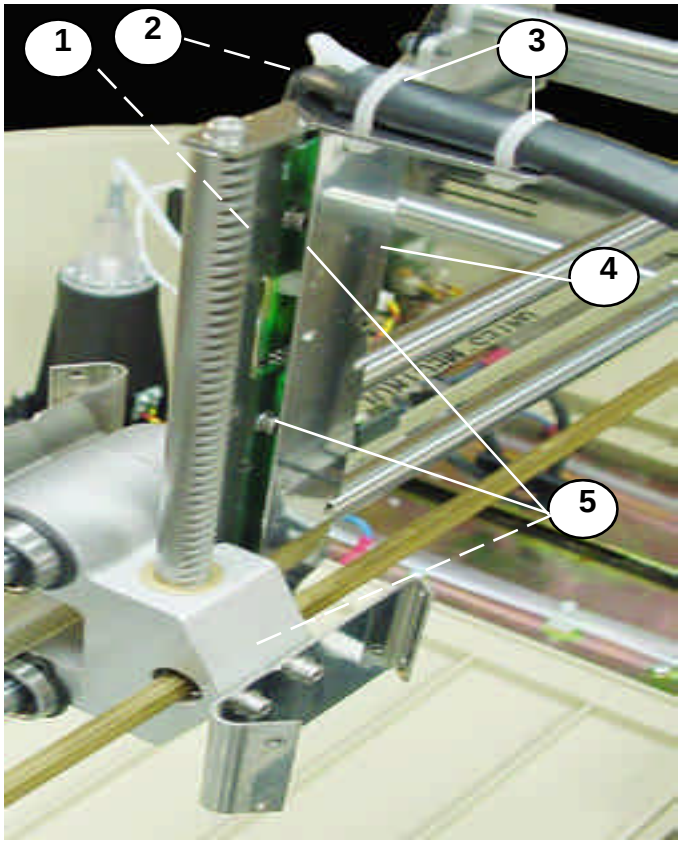

5.1.3.2. Changing the dispensing pump seal

a) Remove the fluidic chamber (1).
b) Remove the washer (2).
c) Replace the seal (3).
d) Refit the washer (2).
d) Refit the fluidic chamber on the pump by tightening the four screws gradually.

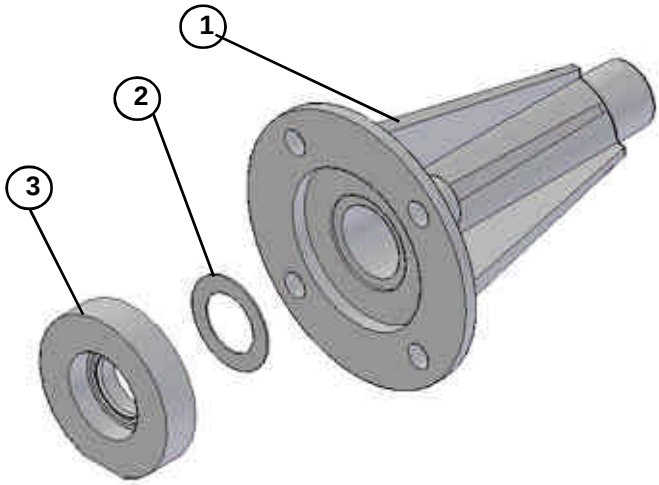

5.1.3.3. Changing the dispensing pump motor

a) Remove the dispensing pump by first of all unscrewing the nuts (1) and then the bolts (2) from the base.
b) Remove the motor by removing the screws (3).
c) Unscrew the body (4).
d) Loosen the Allen bolt and remove the endless screw and the axial bearing (5).
e) Fit the axial bearing and the endless screw on the new motor. The Allen bolt must coincide with the machined surface of the motor axle. Put screwfastener on the bolt. It is very important to remove the axial space between the motor, the bearing and the endless screw. To avoid the displacement of the motor axle, use the MO0009 tool. Tighten the Allen bolt.
g) Clean off the used grease. Put new grease on the endless screw and on the piston support.
h) Clean the piston if it has been stained with lubricant grease.

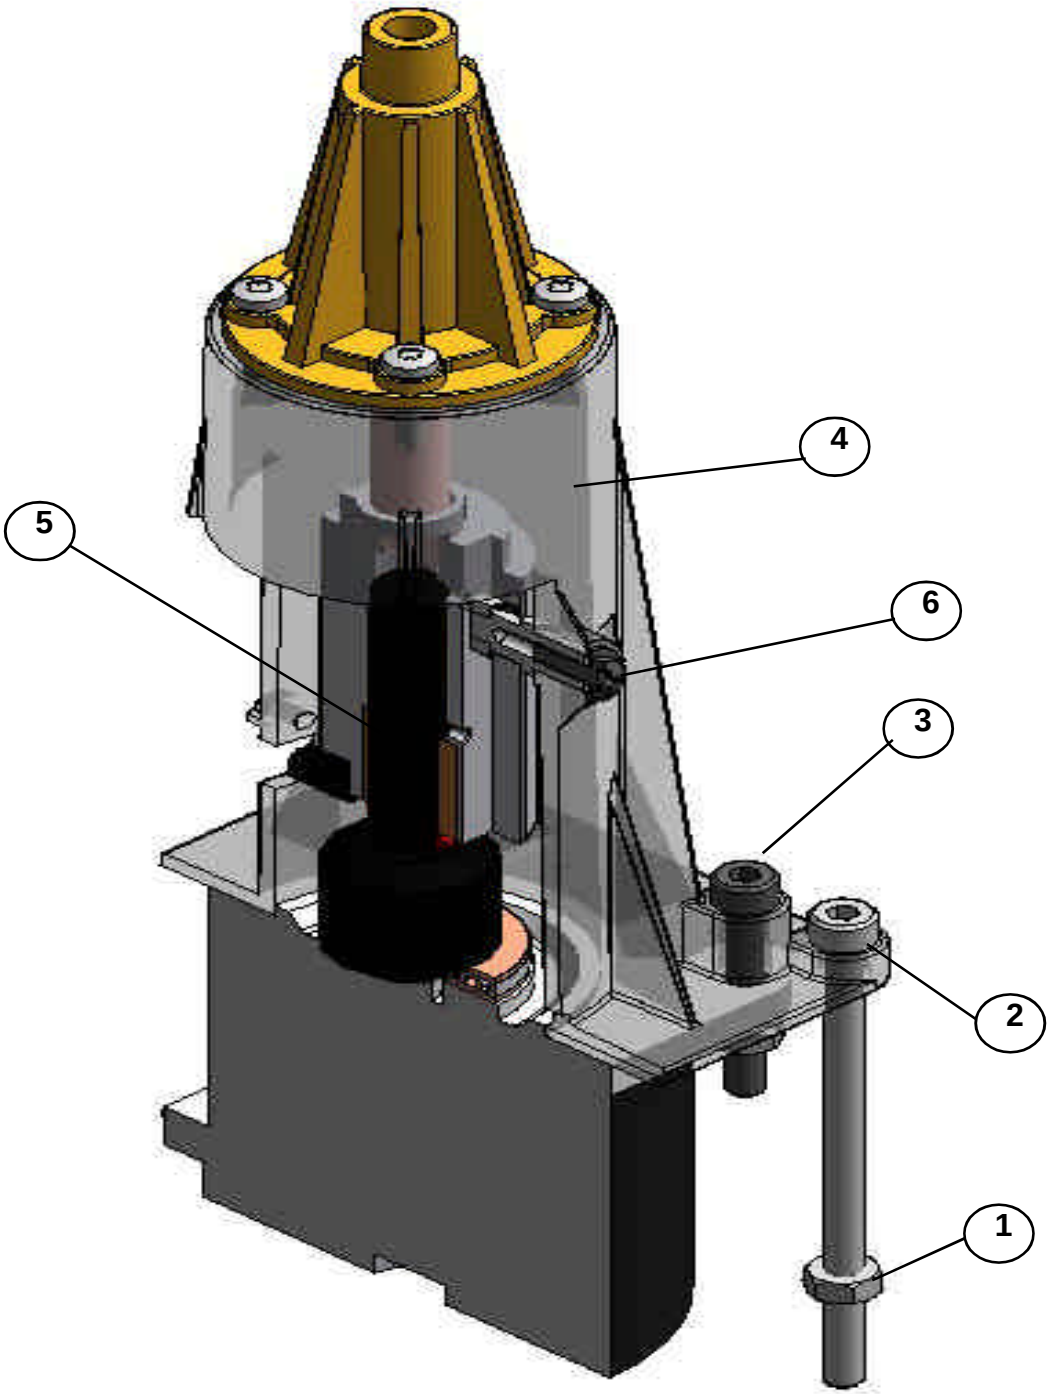

i) Fit the motor with the endless screw and the piston support on the body of the pump, making the support guide coincide with the lock nut (6).
j) Fit the pump to the base. The bolts (2) should not apply pressure to the body (4). Tighten the nuts (2).

5.1.3.4. Changing the dispensing electrovalve

a) Disconnect the connectors (1) and the electrical connector.
b) Remove the screws (2) that hold the electrovalve in position.
c) Fit the new electrovalve. Do not tighten the screws to excess so as not to deform the plastic body of the electrovalve and damage its leakproof quality.
d) When refitting the connectors, use a spanner to tighten them 1/4 of a turn to make sure they are watertight.

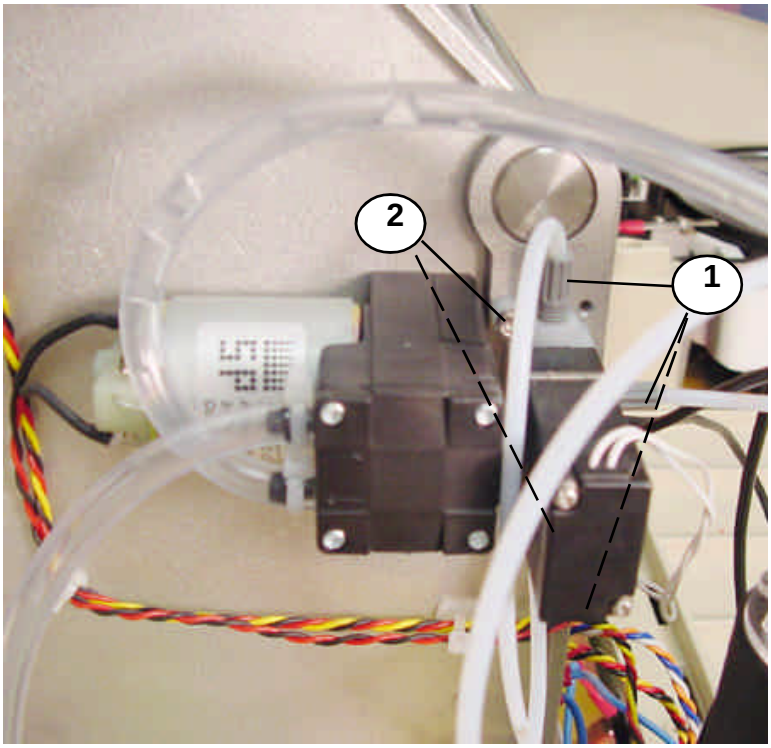

5.1.3.5. Changing the container tube unit

a) Remove the front housing.
b) Disconnect the nuts and the tubes. Remove the grommet from the back housing.
c) Fit the new unit.

5.1.3.6. Changing the distilled water container filters

a) Unscrew the lid and remove the tubes from the distilled water container.
b) Remove the Teflon tube filter by unscrewing the nut.
c) Remove the PVC tube filter by pulling on the filter.
d) Fit the new filters and replace the tubes in the container.

5.1.4. Reactions rotor and reading

5.1.4.1. Changing the rotor temperature probe

a) Remove the upper casing.
b) Disconnect the electrical hose from the interconnection board.
c) Remove the thermal insulation from the temperature probe.
d) Unscrew the probe (2).
e) Clean the thermal silicone form the housing and put fresh thermal silicone on the end of the new probe.
f) Fit the new probe.

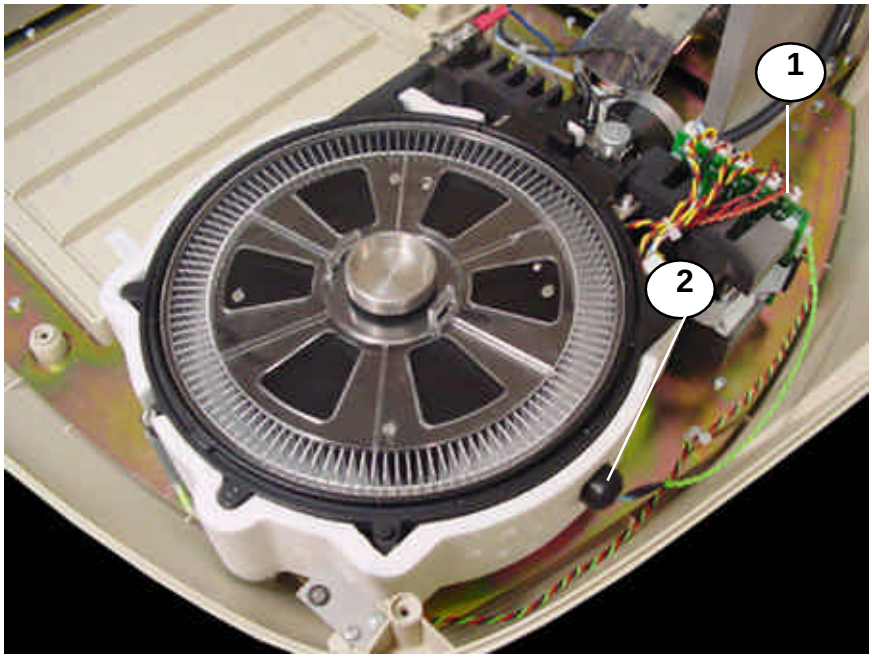

5.1.4.2. Fully removing the rotor

a) Remove the upper casing.
b) Disconnect the electrical hoses and the lampholder (1).
c) remove the rotor from the base by removing the 3 leg screws.

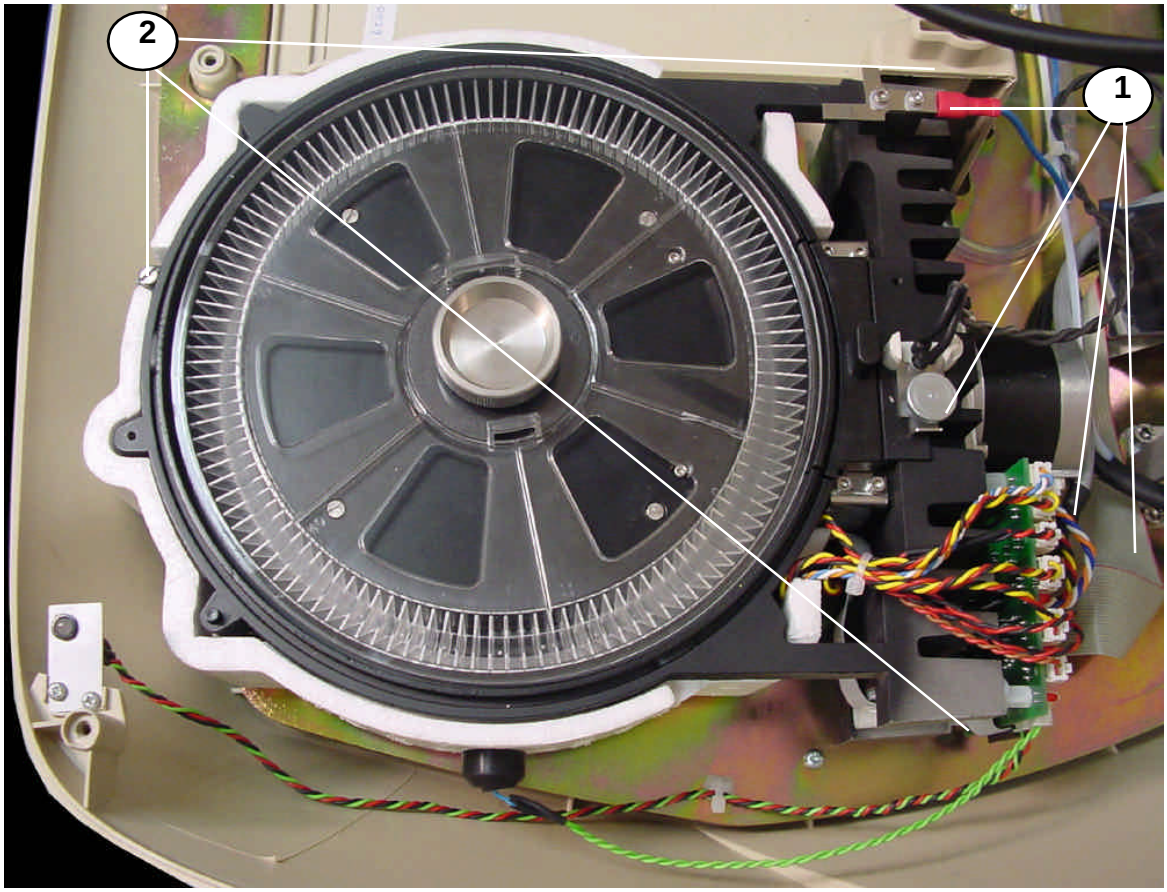

5.1.4.3. Changing the rotor Peltier cells

a) Remove the complete rotor.
b) Remove the bolt (1) and the insulation (2) and the temperature probe (3).
b) Remove the fan (4) and the corresponding radiator (5).
c) Unsolder the Peltier to be replaced and solder the new one in its place. Exactly reproduce the original cabling.
d) Clean the thermal silicone from the heating canal and from the radiator with alcohol. Put fresh thermal silicone on both sides of the new Peltier. Tighten the two bolts equally and apply bolt-fastener.
e) Refit the system.

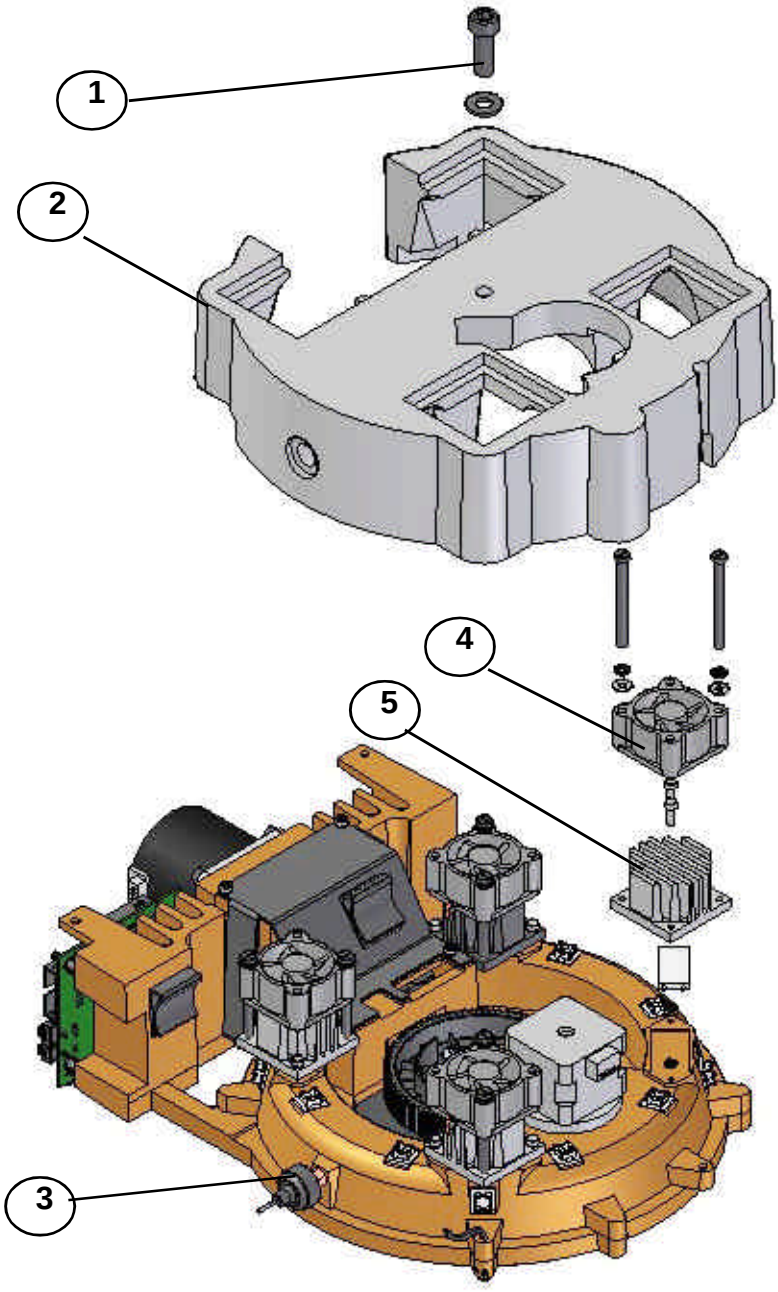

5.1.4.4. Changing the rotor cover detector

a) Remove the rotor completely and remove the insulation.
b) Unscrew the stud (1) and remove the sensor (2).
c) Unsolder the sensor and then solder again.
d) Refit the sensor.

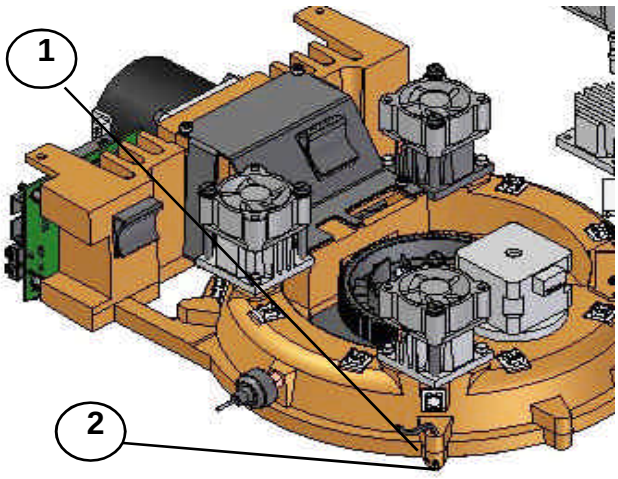

5.1.4.5. Changing the rotor start photosensor

a) Remove the rotor completely and remove the insulation.
b) Remove the start photosensor board (1). Unsolder this board from the electrical hose and solder the new one.
c) Refit the system and check that the centring unit turns freely.

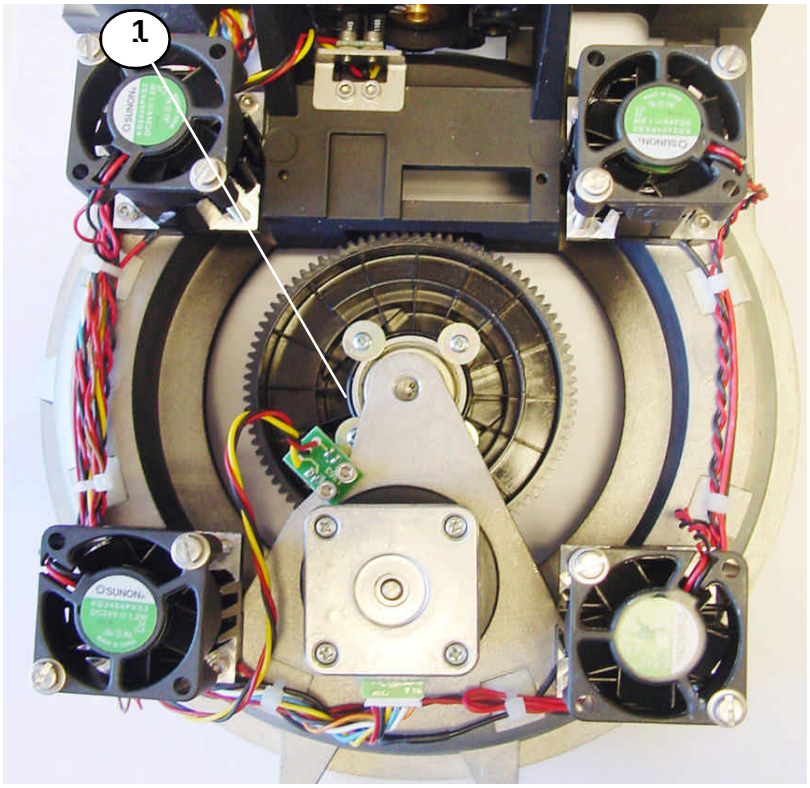

5.1.4.6. Changing the rotor motor

a) Remove the rotor completely. Remove the insulation.
b) Remove the rotor covers.
c) Remove the nuts (1).
d) Remove the motor from below. Disconnect the hose.
e) Fit the new motor on the unit.
f) Perform the miss test on the rotor motor and the rotor positioning test in the service program to check that the gap between gears is correct and that the system functions correctly.

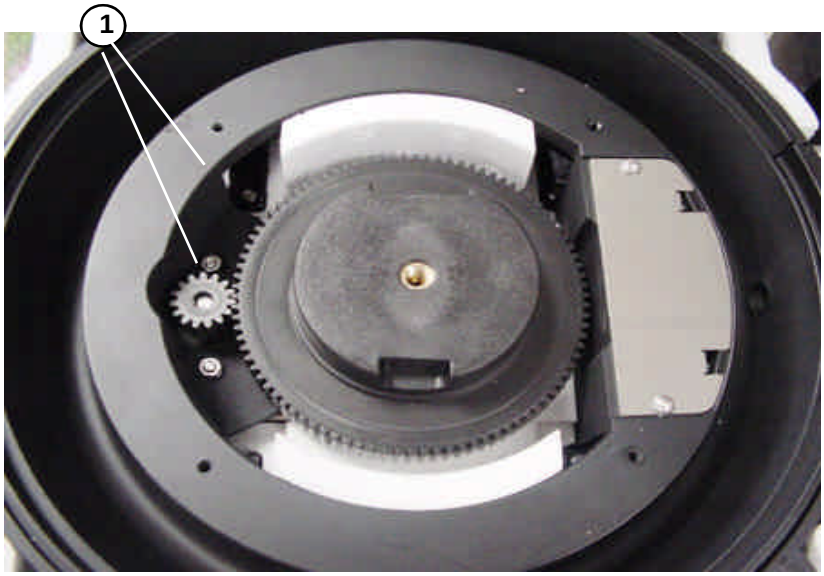

5.1.4.8. Changing the lamp

The analyzer is fitted with a 6 V 10 W halogen lamp with an estimated average lifetime of 2,000 hours. It is recommended that you change the lamp every year even though its lifetime has not run out. When the lamp needs to be changed, access the *Change lamp* utility of the user programme and follow the steps indicated by the programme itself. To replace the lamp, proceed as follows:

a) Remove the rotor cover.
b) Loosen the bolt (1) that holds the fastening tab of the lamp holder in position.
c) Push the tab back.
d) Remove the lamp holder, loosen the Allen screw and take out the lamp.
e) Insert the new lamp, pushing the terminals to the back. Tighten the Allen screw until the lamp is securely in place. Do not touch the lamp bulb with your fingers. To handle the lamp, use the wrapping, cutting it at the terminal end and squeezing it until they come out.
f) Put the lamp holder back in place. Put the tab in position and fasten the bolt (1).
Put the rotor cover back.
ig) The lamp does not require any adjustment, but it can be placed in the analyzer in two possible positions by turning it 180º around its longitudinal axis. The programme itself requires the user to place the lamp in the two possible positions and check in which of the two maximum light intensity is obtained in the optical system.

5.1.4.9. Changing an optical filter

a) Access the *Filter Drum Configuration* screen of the user or service programme. Indicate which filter is to be changed (position 1-9) and click on the *Change filter* button.
b) Remove the rotor cover.
c) Remove the filter drum cover by simply pulling on it.
d) Remove the top filter using a pair of fine pliers.
e) Position the new filter by pressing down until it is correctly in place.
f) Do not leave the position free without putting a filter holder in place. If no filter is required in this position, put a covered filter holder in place.
g) Refit the filter drum cover. Put the rotor cover back.
h) If it is different, introduce the wavelength of the new filter that has been installed.

5.1.4.10. Configuration of the filter drum

a) a) Remove the rotor completely. Remove the insulation.
b) Remove the cover (1).
c) Loosen the Allen bolt that holds the filter drum in place (2).
d) Remove the motor (3). On removing the motor, joined to the drum axle, the drum comes free.
e) Place the new filter drum in position and introduce the motor with the axle in position. The Allen bolt must coincide with the machined area of the axle. Put screwfastener on the bolt.
f) Fit the drum to the axle. Check that the rotor turns freely without mechanical interference.

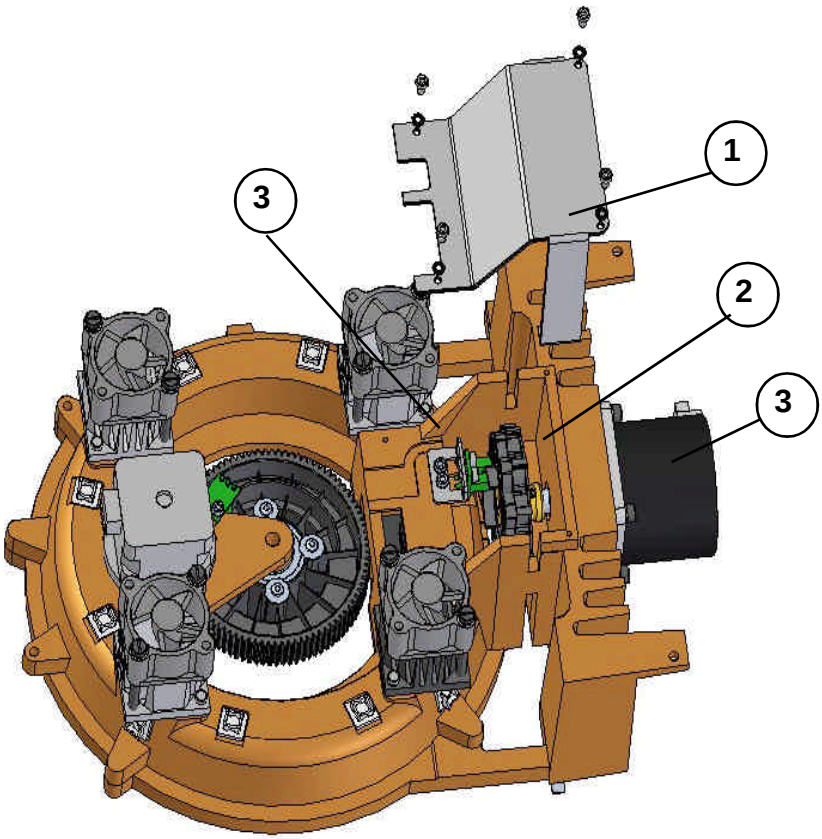

5.1.4.11. Changing the filter drum start photosensor

See the figure in the previous section.

a) Remove the complete rotor.
b) Remove the cover (1).
d) Remove the start photosensor board (3). Unsolder this board from the electrical hose and solder the new one.
e) Refit the system and check that the drum turns freely.

5.1.4.12. Changing the filter drum motor

To change the filter drum motor, proceed as indicated in the section titled Changing the filter drum.

5.1.5. Electronic Systems

5.1.2.1. Changing the X, Y and encoder start photosensor

a) Remove the upper casing.
b) Disconnect all the connectors (1).
c) Remove the protective cover.
d) Disconnect the flat bands (2), cutting the flanges (3).
e) Remove the interconnection board (4).
f) Before connecting the new board, reconnect the flat bands and the flanges.
g) Refit the board and the cover. Fit the casing.

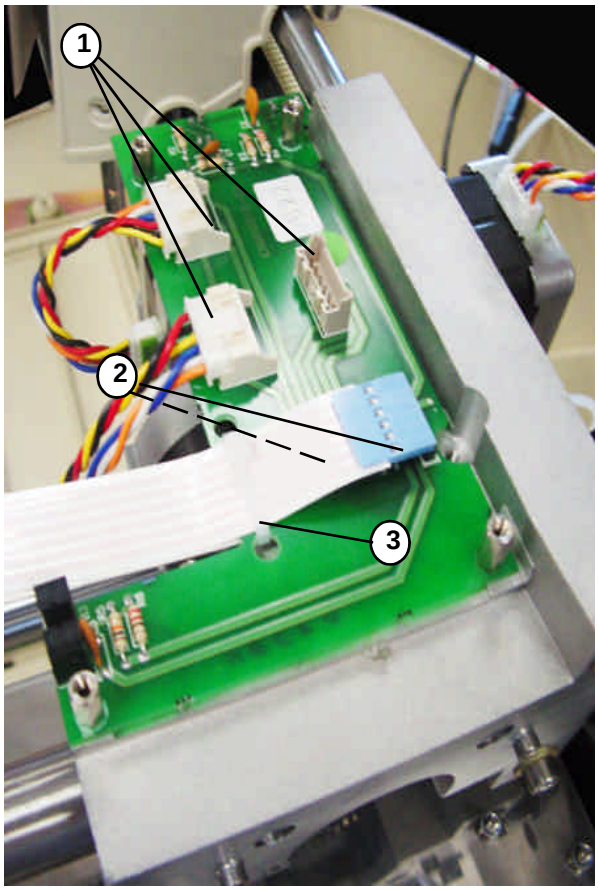

5.1.5.2. Changing the microprocessor board

a) Fold down the back cover of the electronics.
b) Disconnect all the hoses from the board.
c) Remove the bolts (1).
d) When installing the new board, reconnect all the connectors carefully.

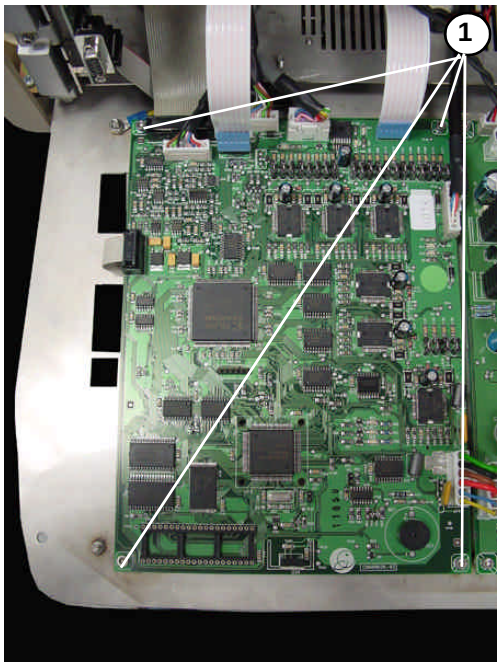

5.1.5.3. Changing the power supply board

a) Fold down the back cover of the electronics.
b) Disconnect all the connectors from the power supply board.
c) Remove the 4 screws (1) that hold the board to the base.
d) Remove the board.
e) When installing the new board, reconnect all the connectors carefully.

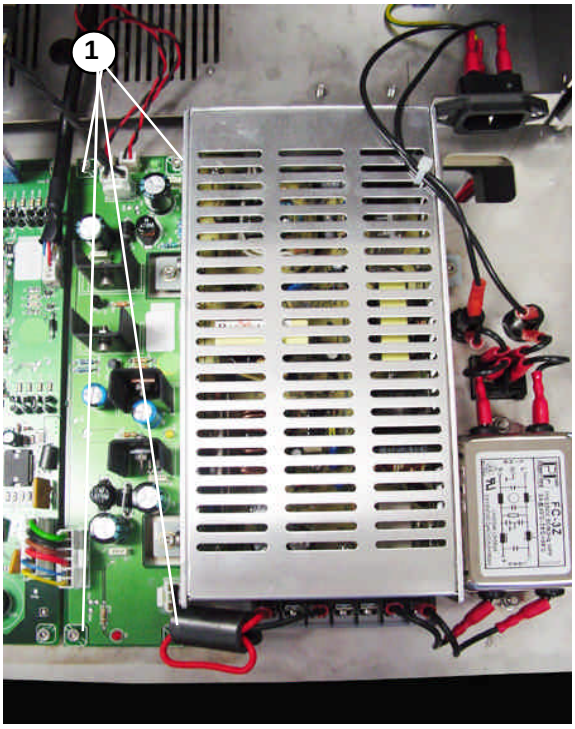

5.1.5.4. Changing the main power supply source

a) Fold down the back cover of the electronics.
b) Remove the input and output connectors by unscrewing the bolts (1).
c) Remove the 3 bolts (2) that hold the source in position.
d) Remove the source.

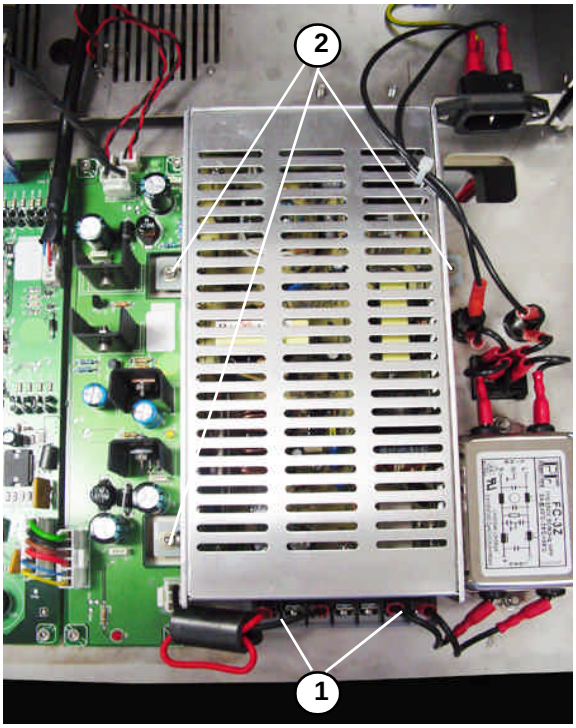

5.1.5.5. Changing the photometric system board

a) Remove the screws from the photometric system support cover.
b) Slightly move the support cover towards the centre of the rotor and remove it from its housing.
c) Disconnect the flat band from the photometric system board.
d) Change the board.
e) Refit the support cover in place ensuring that the flat band is not folded.

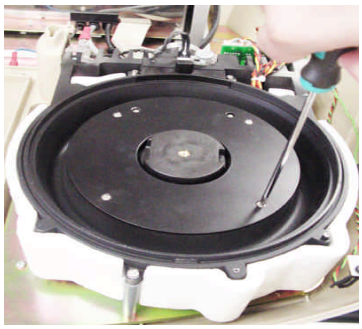

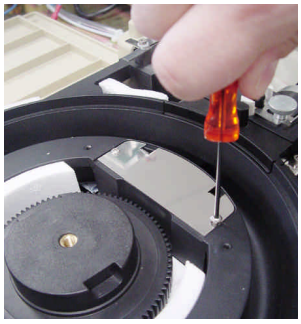

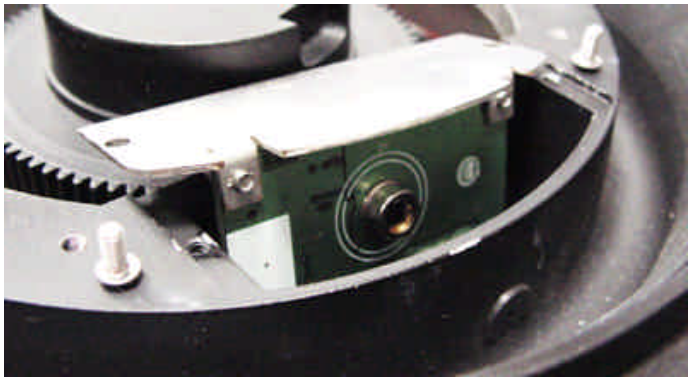

5.1.5.6. Changing the front indicator

a) Remove the upper casing.
b) Disconnect the hose from the rotor interconnection board.
c) Pull the fastening ring (1) down.
d) Pull the LED (2) up to remove it.

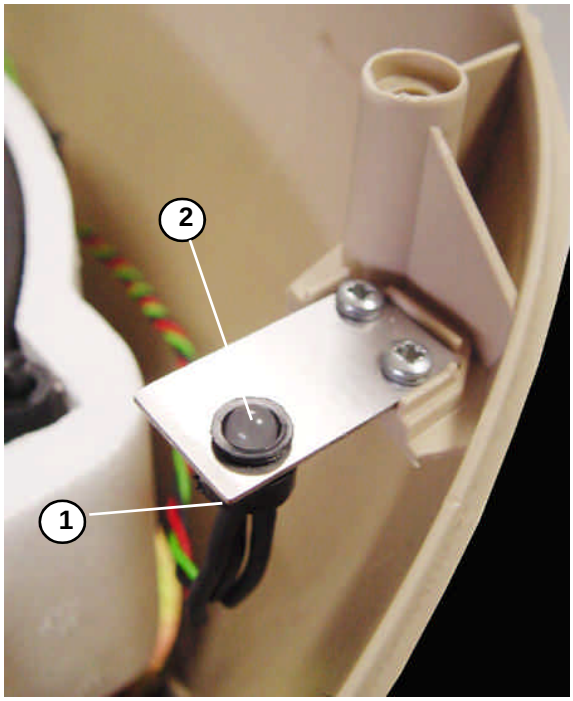

5.1.5.7. Changing the firmware program

The firmware of the analyzer resides in a permanent flash memory. The change of this program can be made through the computer without the need for changing the memory chip. For this, follow the instructions in the section *Loading new firmware versions* of the Service Program.

5.2. RECOMMENDED PREVENTIVE MAINTENANCE

It is recommended that the following maintenance actions are performed annually or every 2,000 working hours.

Operating arm
1. Check the state and tension of the belt.
2. Replace the elements in an unsatisfactory state.
3. Make the adjustments and tests related to the service program.

Dispensing system.
1. Exhaustively wash all the dispensing circuit with washing solution and rinse it with distilled water.
2. Remove and clean the needle. Check its state.
3. Check the state of all the dispensing circuit tubes. Check the absence of obstructions or diameter changes.
4. Check the leakproof quality of the nuts and the 3-channel electrovalve body.
5. Check the leakproof quality of the dispensing pump nut and seal. Check there is no loss and no bubbles. Change the seal every 2 years.
6. Clean the distilled water container filters.
7. Clean the washing station.
8. Check the state of the washing system tubes.
9. Replace the elements in an unsatisfactory state.
10. Make the adjustments and tests related to the service program.

Reactions rotor
1. Check the state of the heating canal.
2. Verify the gap betwen gears.
3. Replace the elements in an unsatisfactory state.
4. Make the adjustments and tests related to the service program.

Optical system
1. Check the state of the lamp. Check if it has been working for over 1,000 hours.
2. Clean the filters.
3. Clean the photodiode.
4. Replace the elements in an unsatisfactory state.
5. Make the adjustments and tests related to the service program.

5.3. CARE AND CLEANING

5.3.1. General care of the analyzer

a) Never use detergents or abrasive products for cleaning the surface of the analyzer. Use only a damp cloth with water and pH-neutral soap.
b) If a reagent or corrosive product spills or splashes onto the apparatus, clean it with a damp cloth and soap immediately. If necessary, protect your hands with appropriate laboratory gloves.
c) All the elements of the analyzer have drainage conduits leading to the exterior to enable the elimination of any liquid spilled and to prevent the apparatus from flooding. If the spillage is significant, the liquid spilled onto the table through the drainage conduits and the analyzer must be adequately cleaned.
d) When not in use, close the main cover of the analyzer to protect it from dust.

5.3.2. Cleaning the optical system

The components of the optical system must be cleaned periodically in order to keep them free from dust and dirt. These components are the lamp, the filters and the photodiode. The recommended necessary material is as follows:

- Special paper for cleaning optical components (non-abrasive paper which does not leave solid residue).
- Ether and alcohol solution at 50%
- Cotton wool buds.
- Small bellows.

All the optical elements must be handled in an area of maximum cleanliness, given that they are fragile and delicate. To remove them and refit them, the corresponding instructions given in the *Maintenance* chapter must be carefully followed. Avoid touching the useful area of these elements with fingers. The filters and the photodiode must be held by the sides. Do not touch the lamp bulb. To handle the lamp, use the wrapping, cutting it at the terminal end and squeezing it until they come out. To clean the optical components, bear in mind the following:

a) Remove the dust on the surface of the component with the bellows. This will avoid scratching by particles when cleaning with paper.
b) Carefully clean the surface of the component with the cleaning paper.
c) If the dirt is persistent or greasy, clean the component with the paper moistened with the alcohol and ether solution. Then dry with dry paper. To clean the filters or the window of the photodiode, use the cotton wool buds with the paper in difficult and delicate areas.
d) Finally, it is recommended that you use the bellows once again, thus removing any remains of paper or cotton.

5.3.3. Cleaning the dispensing system

It is a good idea to recommend to the user that he configures the analyzer to automatically wash the dispensing system with washing solution at the start and end of each working day to ensure that it is completely free from air bubbles and is perfectly clean. With the initial wash, the system is ready for working in optimum conditions during the entire working day, offering maximum performance. With the final wash, the analyzer cleans the needle at the end of the working day, keeping it in optimum condition for future working days. Additional washing of the dispensing system can be performed using the *Dispensing system wash* utility of the user program. The analyzer must be in standby mode.

The user himself should clean and check the state of the distilled water container filters at least once every 3 months. The service operations should also check the state of these filters.

If the needle is obstructed by solid residue, it must be removed and cleaned using the metal cleaning rod supplied with the analyzer. For this, the *Remove the dispensing needle* utility should be used. It is also recommendable to clean the outside surface of the needle with a piece of cotton or a soft cloth dampened with alcohol. The needle must be replaced if it noticeably deteriorates.

5.3.4. General cleaning of the interior of the apparatus

It is important for the interior of the instrument to be free from dust at all times in order to preserve the correct functioning of the different elements. For this, remove the front housing of the analyzer and electronics cover and carefully clean the dust inside the instrument.

A I. TECHNICAL SPECIFICATIONS

PLEASE NOTE
The manufacturer accepts no liability for damage caused by incorrect use of the apparatus.

GENERAL SPECIFICATIONS

Automatic random and continual access analyzer aimed at giving results per patient, with direct photometric reading over a reactions rotor.

Preparation cycle time	24 s (up to 150 prep/h)
Warm-up time	25 mins
Reading time for each preparation	Every 24 s, up to 10 mins
Dimensions	840 x 670 x 615 mm (33.1"x26.8"x24.2") (length x depth x height)
Weight	45 kg (100lb)

REAGENTS AND SAMPLES TRAY

Positions for racks	4
Capacity of the sample racks	24
Maximum number of samples	72
ø13 mm, ø15 mm sample tubes (max. height 100 mm),	ø13 mm paediatric well
Capacity of the reagent racks	10
Maximum number of reagents	30
20 ml and 50 ml reagent bottles	
Possible configurations	

Sample racks	Reagent racks	Number of samples	Number of reagents
1	3	24	30
2	2	48	20
3	1	72	10

DISPENSING SYSTEM

NEEDLE

Detachable tip	
Vertical length	110 mm
Capacity level detection	
Self-adjustment of position	

NEEDLE THERMOSTATATION SYSTEM

Actuator	Resistive elements
Control	PID
Thermostatation time	$\leq$ 15 s
Dispensation temperature	37°C
Trueness	± 0.5°C
Repeatability	± 0.5°C

DISPENSING PUMP

Ceramic piston with PTFE-graphite seal	
Piston diameter	8 mm
Displacement	25 mm
Dispensing volume	3 µL - 1250 µL
Resolution	0.126 µL
Fuzziness	<1% up to 3 µL
Dispensing speed	max. 880 µL/s
Programmable reagent volume	10 µL -440 µL
Programmable sample volume	3 µL - 40 µL

NEEDLE WASHING SYSTEM

System liquid consumption	approx. 2.4 ml per preparation
System liquid container volume	3000 ml
Waste container volume	3000 ml
Capacitance waste and water level control	

REACTIONS ROTOR AND READING

WELL ROTOR

Semi-disposable extractable methacrylate rotor	
Number of wells	120
Accepted reaction volumes	200 µL - 800 µL
Light path length	6 mm

ROTOR THERMOSTATATION SYSTEM

Actuators	4 Peltier cells
Control	PID
Working temperature	37°C
Trueness	± 0.2°C
Stability	± 0.1°C

OPTICAL SYSTEM

Halogen lamp	6 V, 10 W
Wavelength selection with compensated interferential filters	
Detection system with silicon photodiode and 20-bit AD integrator-converter	
Measurement range	from -0.05 A to 2.5 A
Reading speed	1.25 readings/s
Maximum number of filters	9
Base configuration of the filter drum	340, 405, 505, 535, 560, 600, 635, 670 nm
Wavelength precision	± 2 nm
Bandwidth	10 ± 2 nm
Digital resolution	$\underline{<}$ 0.0001 A
Base line stability	max. 0.004 A in 30 mins, at 505 nm
Repeatability of the reading system (1 SD, 505 nm, with filter movement)	± 0.0005 A to 0.1 A (CV = 0.5%) ± 0.0003 A to 1.0 A (CV = 0.3 %) ± 0.0005 A to 2.5 A (CV = 0.2 %)
Optical repeatability between wells	± 0.003 A at 340 nm ± 0.002 A to 505 nm, 670 nm
Precision	± 0.005 A to 0.1 A (± 5%) ± 0.015 A to 0.5 A (± 3%) ± 0.02 A to 1.0 A (± 2%) ± 0.04 A to 2.0 A (± 2%) ± 0.05 A to 2.5 A (± 5%) at 340 nm, 405 nm, 505 nm

MINIMUM COMPUTER REQUIREMENTS

Pentium IV processor or higher
Windows 98 or higher
256 Mb RAM
50 Mb free hard disk space
CD-ROM
VGA Monitor, minimum resolution of 640x480
Mouse
RS-232 serial channel or USB connector
The insulation level of the communications channel of the A15 analyzer is *reinforced* (the insulation of the communications channel of the computer must also be reinforced)(1)

POWER REQUIREMENTS

Input voltage	125-230 Vac, 50/60 Hz
Power	150 VA
Electrical installation category (overvoltage category)	II
The power point must be officially approved, earthed and the cable must have a minimum cross-section of 1.5 $mm^{2.}$	

ATMOSPHERIC CONDITIONS

Interior use	
Height	< 2500 m
Temperature	10°C - 35°C
Relative humidity	< 75%
Contamination level	2

(1) Reinforced insulation is that which ensures protection equal to or higher than double that provided by the main insulation.
The main insulation is that whose failure could lead to a risk of electric shock *(EN 61010-1).*

COMPLIANCE WITH DIRECTIVES AND APPLIED STANDARDS

Directive 98/79/CEE regarding sanitary products for *in vitro diagnostic* use

- EN 61010-2 -10:2002 “Safety requirements for electrical equipment for measurement, control and laboratory use. : EN61010-2-101:2004»Particular requirements for vitro diagnostics(IVD) medical equipment”
- UNE EN 61326:1999+A1:2000+A2:2003+A3:2005+ERR:2002 “Electromagnetic equipment for measurement, control and laboratory use –ECM requirements.
  - UNE-EN 55022:2000+A1:2002+CORR:2002- Radiated emissions class B-continuous interference class B”.
  - UNE -EN 61000-3-2:2002 «Harmonic current»
  - UNE -EN 61000-3-3:1997+Corr:1999+A1:2002-»Flickers»
  - UNE -EN 61000-4-2:1997+A1:1999+A2:2001
  - UNE -EN 61000-4-3:2003+A1:2004-»Radiated immunity»
  - UNE -EN 61000-4-4:1997+A1:2001+A2:2002-»Fast transient /Burst»
  - UNE -EN 61000-4-5:1997+A1:2001-»Surge transients»
  - UNE -EN 61000-4-6:1998+A1:2001-»Conducted immunity»
  - UNE -EN 61000-4-11:1997+A1:2001-»Voltage disp short interruptions and voltage variations immunity»
- UNE EN 22233-02. Test packaging.
- UNE EN 24180-2.Complete and full shipment packaging.
- UNE EN 22247-03(ISO 2247-2000). Fixed low frequency vibration test.
- UNE EN 22248-94. Freefall vertical shock test.

MAXIMUM SIZE OF ANALYZER

With the lid closed:	Width: 840 mm.	Depth: 670 mm.	Height: 615 mm.
With the lid open:	Width: 840 mm.	Depth: 670 mm.	Height: 1,025 mm.

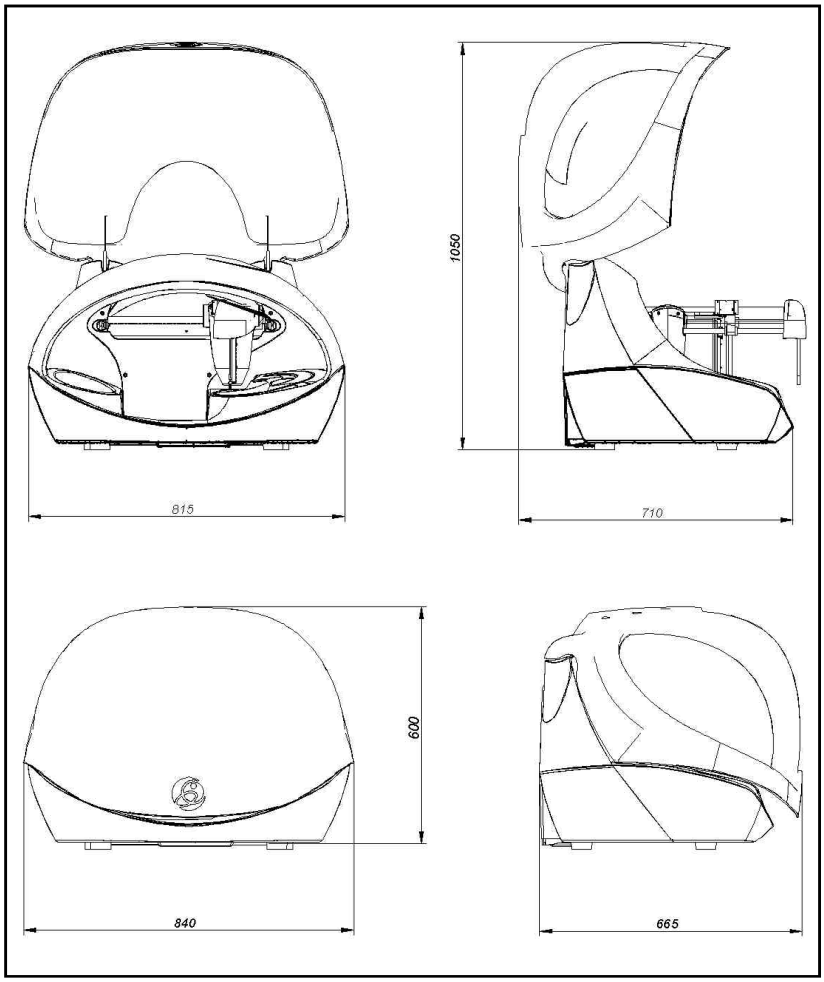

The manufacturer reserves the right to modify any technical specification without prior notice.

A II. ADJUSTMENT MARGINS TABLES

Main voltage measurement points

CIIM0015 Power supply board

TP1 - 6V	[5.6-5.8] V
TP2 - 12V	[11.7 -11.9] V
TP3 - 5V	[4.9-5.2] V
Sp150	[23.5-24.5] V

CIIM0026 Microprocessor board

TP60 - Vref motor Z	[13 -15] mV
TP61 - Vref motor Y	[13 -15] mV
TP56 - Vref motor X	[13 -15] mV
TP57 - Vref pump motor	[13 -15] mV
TP58 - Vref filter motor	[13 -15] mV
TP59 - Vref rotor motor	[13 -15] mV

Main adjustment values of the analyzer

	Tolerances
Operating arm positioning	
X axis loss of steps	
Loss of steps	[-3,3]
Y axis loss of steps	
Loss of steps	[-3,3]
Z axis loss of steps	
Loss of steps	[-3,3]
Loss of steps rotor motor	
Loss of steps	[-3,3]
Loss of steps filter drum motor	
Loss of steps	[-3,3]
Loss of steps pump motor	
Loss of steps	[-4,4]
XY position adjustment	
X origin	[10,125]
Y origin	[240,290]
X racks tray	[620,750]
Y racks tray	[-20,20]
X washing station	[330,450]
Y washing station	[70,120]
X rotor	[60,170]
Y rotor	[1030,1060]
Maximum Z	[1090,1155]
Self-centering of needle	
X Offset	[-4,4]
Y Offset	[-4,4]
Bottle level control sensitivity	
Water empty	[200,255]
Water full	[30,120]
Water calculated	[85,160]
Waste empty	[200,255]
Waste full	[25,140]
Waste calculated	[90,175]
Level detection sensitivity	
Paediatric rack	[15,60]
13/15mm tube sample rack	[15,60]
Reagent rack	[9,35]
Positioning of the dispensing point	
Dispensing rotor	[90,120]
Fine rotor X	[35,200]
Needle thermostatation	
Set point temperature	[35,41]
Rotor thermostatation	
Set point temperature	[36,37.5]
Filter drum positioning	
Positioning	[-5,5]
Positioning of rotor in optic	
Positioning	[-15,0]
Integration times	
F1 340 nm	[190,350]
F2 405 nm	[40,130]
F3 505 nm	[40,130]
F4 535 nm	[40,130]
F5 560 nm	[40,130]
F6 600 nm	[40,130]
F7 635 nm	[40,130]
F8 670 nm	[50,130]
Number of counts	
F1 340 nm	[750000,970000]
F2 405 nm	[840000,970000]
F3 505 nm	[840000,970000]
F8 670 nm	[840000,970000]
Darkness counts	
F1 340 nm	[3700,4300]
F2 405 nm	[3700,4300]
F3 505 nm	[3700,4300]
F8 670 nm	[3700,4300]
SMF repeatability (Noise)	
Dev. Est. NC. F0 Covered	≤ 55
Dev. Est. Abs. F1 340 nm	≤ 0.0004
Dev. Est. Abs. F2 405 nm	≤ 0.0006
Dev. Est. Abs. F3 505 nm	≤ 0.0004
Dev. Est. Abs. F8 670 nm	≤ 0.0007
Stability at 505 nm	
Dev. Est. Abs. F3 505 nm	≤ 0.0008
Max. NC	[840000,970000]
Min. NC	[840000,970000]
Max NC / Min NC	≤ 1,006
Repeatability MF (Repeatability)	
Dev. Est. Abs. F1 340 nm	≤ 0.0008
Dev. Est. Abs. F2 405 nm	≤ 0.0006
Dev. Est. Abs. F3 505 nm	≤ 0.0005
Dev. Est. Abs. F4 535 nm	≤ 0.0005
Dev. Est. Abs. F5 560 nm	≤ 0.0005
Dev. Est. Abs. F6 600 nm	≤ 0.0005
Dev. Est. Abs. F7 635 nm	≤ 0.0005
Dev. Est. Abs. F8 670 nm	≤ 0.0005

A III. LIST OF CONSUMABLES, ACCESSORIES AND SPARES

If any of the components of the analyzer deteriorate of if any of the perishable materials are required, always use original BioSystems material. The following table shows lists of components that may be required. To purchase said components, please contact your usual distributor and order each element using its corresponding code. This will simplify work and minimise errors.

List of user spares, perishable materials and accessories.

CODE	DESCRIPTION (Ordered by code)
CA10455	European network cable
CA10456	American network cable
FI10466	Serial channel cable for connection to PC
AC10770	Sample wells (1000),Paediatric reaction wells
AC11485	Reaction rotor (10 units)
AC11486	Reactions rotor fastening screw
FI11490	535 nm filter unit
FI11491	560 nm filter unit
BO1149	350 ml bottle with top (10 units)
BO1149	420 ml bottle with top (10 units)
FI11498	Covered filter unit
AC11501	20 ml/50 ml reagents rack
AC11502	13 mm tube sample rack
AC11503	15 mm tube sample rack
AC11504	Paediatric well samples rack
BO11524	Bottle of concentrated system liquid (1L)
FI11563	340 nm filter unit
FI11564	405 nm filter unit
FI11565	505 nm filter unit
FI11566	600 nm filter unit
FI11567	635 nm filter unit
FI11568	670 nm filter unit
AC12222	Metal rod for cleaning the needle
AC12223	2 mm Allen key
BO13146	Concentrated washing solution (100mL)
AC13188	User programme CD
BO13189	System liquid container with top
FI13190	System liquid container filters
BO13191	Washing solution container with top
BO13192	Waste container with lid and fitting
AC13193	Detachable needle
FU13194	Set of 2 A (F) fuses
LA13195	6 V/10 W halogen lamp
ZO13196	Lamp holder fastening system
AC13197	Reactions rotor cover
AC13198	Operating arm fastening for transport (screw and foam)
AC13199	Height-adjustable leg
AC13200	Filter drum cover
	User Manual/Installation and maintenance manual

CODE	DESCRIPTION (Ordered by description)
AC11502	13 mm tube sample rack
AC11503	15 mm tube sample rack
AC12223	2 mm Allen key
BO11494	20 ml bottle with top (10 units)
AC11501	20 ml/50 ml reagents rack
FI11563	340 nm filter unit
FI11564	405 nm filter unit
BO11493	50 ml bottle with top (10 units)
FI11565	505 nm filter unit
FI11490	535 nm filter unit
FI11491	560 nm filter unit
LA13195	6 V/10 W halogen lamp
FI11566	600 nm filter unit
FI11567	635 nm filter unit
FI11568	670 nm filter unit
CA10456	American network cable
BO11524	Bottle of concentrated system liquid (1L)
BO13146	Concentrated washing solution (100mL)
FI11498	Covered filter unit
AC13193	Detachable needle
CA10455	European network cable
AC13200	Filter drum cover
AC13199	Height-adjustable leg
ZO13196	Lamp holder fastening system
AC12222	Metal rod for cleaning the needle
AC13198	Operating arm fastening for transport (screw and foam)
AC11504	Paediatric well samples rack
AC11485	Reaction rotor (10 units)
AC13197	Reactions rotor cover
AC11486	Reactions rotor fastening screw
AC10770	Sample wells (1000), Paediatric reaction wells
FI10466	Serial channel cable for connection to PC
FU13194	Set of 2 A (F) fuses
FI13190	System liquid container filters
BO13189	System liquid container with top
	User Manual/Installation and maintenance manual
AC13188	User programme CD
BO13191	Washing solution container with top
BO13192	Waste container with lid and fitting

List of spares exclusive to the technical support service.

CODE	DESCRIPTION (Ordered by code)
CA13308	CD-ROM with Service programme and Service manual
VA10355	Mains connector
ZO10407	Fuse holder
IN11557	Mains switch
FO11570	Set of five photosensors
AC11860	Temperature adjustment tool
AC13350	Full operating arm
MO13351	X guide motor
ME13352	Y carriage belt
MO13353	Y guidemotor
MO13354	Z guide motor
ME13355	Spring set
AC13356	Full thermostated needle set
MO13357	Peltier fan
MO13358	A15 fan
ME13359	Full dispensing pump
AC13360	Thermostated needle fastening nut
AC13361	Dispensing pump seal
AC13362	Dispensing pump fluid chamber
MO13363	Dispensing pump motor
ME13364	Electrovalve
AC13365	Arm hose
TU13366	Container tube unit
ME13367	Waste pump
TU13368	PVC waste tube
AC13369	Waste container nut and cap
AC13370	Full reactions rotor
AC13371	Rotor temperature sensor
MO13372	Rotor motor
AC13373	Rotor cover sensor
ZO13374	Lamp holder
AC13375	Filter wheel body
MO13376	Filter wheel motor
ME13377	Hydro-pneumatic cylinder of the cover hinge
CA13378	Upper cover of needle set
CA13379	Bottom cover of needle set
PC13380	Microprocessor board
PC13381	Photometric system board
PC13382	Front indicator
PC13383	Power supply board
PC13384	Communications board
PC13385	XYZ interconnection board
PC13386	Rotor interconnection board
PC13387	Pumps interconnection board
CE13388	Peltier cell
TR13389	Main power supply
CA13393	Base cover
CA13394	Upper cover
CA13395	Front al cover
CA13396	Spring protection cover
CA13397	Instrument cover

CODE	DESCRIPTION (Ordered by description)
MO13358	A15 fan
AC13365	Arm hose
CA13393	Base cover
CA13379	Bottom cover of needle set
PC13384	Communications board
TU13366	Container tube unit
AC13362	Dispensing pump fluid chamber
MO13363	Dispensing pump motor
AC13361	Dispensing pump seal
ME13364	Electrovalve
AC13375	Filter wheel body
MO13376	Filter wheel motor
PC13382	Front indicator
CA13395	Front al cover
AC13356	Full thermostated needle set
ME13359	Full dispensing pump
AC13350	Full operating arm
AC13370	Full reactions rotor
ZO10407	Fuse holder
ME13377	Hydro-pneumatic cylinder of the cover hinge
CA13397	Instrument cover
ZO13374	Lamp holder
TR13389	Main power supply
VA10355	Mains connector
IN11557	Mains switch
PC13380	Microprocessor board
MO13357	Peltier fan
CE13388	Peltier cell
PC13381	Photometric system board
PC13383	Power supply board
PC13387	Pumps interconnection board
TU13368	PVC waste tube
AC13373	Rotor cover sensor
PC13386	Rotor interconnection board
MO13372	Rotor motor
AC13371	Rotor temperature sensor
CA13308	CD-ROM with Service programme and Service manual
FO11570	Set of five photosensors
CA13396	Spring protection cover
ME13355	Spring set
AC11860	Temperature adjustment tool
AC13360	Thermostated needle fastening nut
CA13394	Upper cover
CA13378	Upper cover of needle set
AC13369	Waste container nut and cap
ME13367	Waste pump
MO13351	X guide motor
PC13385	XYZ interconnection board
ME13352	Y carriage belt
MO13353	Y guidemotor
MO13354	Z guide motor

A IV. LIST OF REQUIRED TOOLS

1. Set of metric Allen keys.
2. Loctite 243 screwfastener or similar
3. Mechanical grease ELESA NT1 (for ceramic pump only) (AC13079).
4. Heat silicone or similar
5. Soldering iron
6. Screwdrivers or two 3 mm Allen keys.
7. Loctite 245 or similar (for ceramic pump only).
8. Temperature adjustment tool (AC11860).

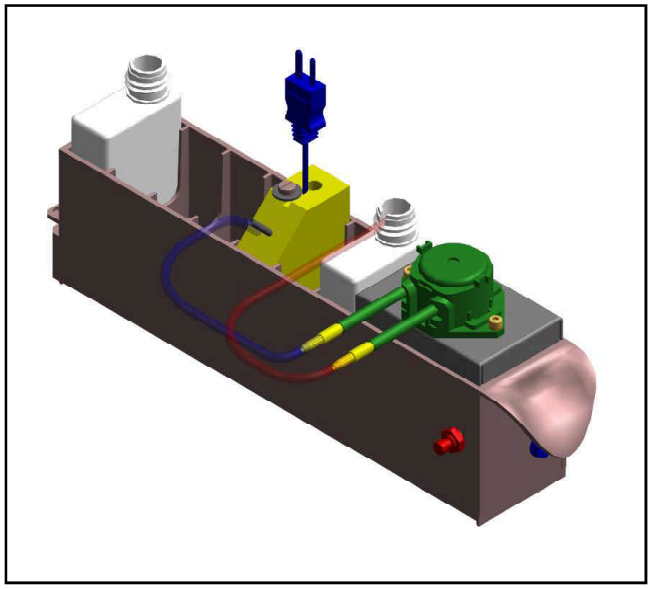

Temperature adjustment tool

A V. SOFTWARE VERSIONS

Change in the versions of service program

Date	version	Change
04/04/06	3.0.1	First release version
20/07/06	3.0.2	Correction of errors Improve the checking before load a new firmware
18/12/06	3.1.0	Modify the level sensitivity adjustment screen to incorporate the independent adjustment by type of rack. Added the help menu with the preventive maintenance guide.

Change in the versions of user program

Date	version	Changes
04/04/06	3.2.1	First release version
20/07/06	3.2.2	New button in the tools menu, reset the historical base line Fix the options of the initial and final wash. Delete the menu to choose the parameter of initial and final wash. Add a maintenance guide in the help menu.
14/11/06	3.3.0	Improve and optimitation of the execution times of the application. Corrected the application errors that showed the message «not respond»
05/03/07	3.3.1	Korean language included

Change of some test adapters
Correction of low frequency errors

Change in the versions of firmware

Date	version	Change
04/04/06	2.90	First release version
09/05/06	2.92	Improvements in the generation of the pattern of encoder
18/12/06	3.10	In order to avoid the splashes in the dispensation of the predilution, the dispensation speed have been reduced. The sensitivity adjustment have been split in 3 diferents adjustments, one for each type of rack.
6/02/07	3.12	Increase the stabilization time of the commutation of 3 way electrovalve.
07/03/07	3.14	Correction: when shut-down is made and next the warming-up without disconnecting the analyzer the termostatización of the probe does not activate.

Compatibilities table

User A25 firmware	3.2.1	3.2.2	3.3.0	3.3.1
2.90	x	x	x	x
2.92	x	x	x	x
3.10	x	x	x	x
3.12	x	x	x	x
3.14	x	x	x	x

It is advisable to always install the last existing version of firmware.

BIOSYSTEMS, S.A. Costa Brava, 30, 08030 Barcelona - Spain Tel: 34-93 311 08 11 Fax: 34-93 346 77 99
*e-mail:*biosystems@biosystems.es http://www.biosystems-sa.com